



Deposited via The University of Leeds.

White Rose Research Online URL for this paper:

<https://eprints.whiterose.ac.uk/id/eprint/102390/>

Version: Accepted Version

Conference or Workshop Item:

Maqbool, HF, Husman, MAB, Awad, MIMH et al. (2015) Real-time gait event detection using a miniature gyroscope to improve rehabilitation for artificial lower limb users. In: 2015 IEEE/RSJ International Conference on Intelligent Robots and Systems (IROS).

Reuse

Items deposited in White Rose Research Online are protected by copyright, with all rights reserved unless indicated otherwise. They may be downloaded and/or printed for private study, or other acts as permitted by national copyright laws. The publisher or other rights holders may allow further reproduction and re-use of the full text version. This is indicated by the licence information on the White Rose Research Online record for the item.

Takedown

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing eprints@whiterose.ac.uk including the URL of the record and the reason for the withdrawal request.

Real-time gait event detection using a miniature gyroscope to improve rehabilitation for artificial lower limb users*

H. F. Maqbool, M. A. B. Husman, M. I. Awad, A. Abouhossein, and A. A. Dehghani-Sanij

Abstract— This paper presents a simple heuristic rule based on real-time gait event detection algorithm for transfemoral amputees based on gyroscope signal and validate with footswitches for ramp activities with different inclination.

I. INTRODUCTION

Accurate detection of human gait events such as initial contact (IC) and toe off (TO) and/or phases is vital in gait analysis and has important applications in assistive devices such as prosthetics/orthotics for rehabilitation purposes [1]. Among wearable sensors, gyroscopes are being widely used for long term monitoring of ambulatory systems. Less soft tissue movement on the anterior side of the shank than thigh and less signal variability between the subjects compared with foot signal are primarily the main advantages of attaching gyroscope on shank [2]. This study presents a simple algorithm for event detection and evaluated on transfemoral amputee for two inclined surfaces (5° and 8.4°).

II. EXPERIMENTAL SETUP AND ALGORITHM DESCRIPTION

A gyroscope and a base unit containing circuitry and battery unit were placed on the anterior side of the shank with the help of Velcro straps. For validation purposes, an insole consisting of four footswitches located at the heel, 1st and the 5th metatarsals and toe was placed inside the shoe shown in Fig.1. One transfemoral amputee (age: 53 years old; weight: 66.7 Kg; height: 166.1 cm) who uses Orion2 (knee) and echelon (foot) with no other neurological problems other than his amputation participated in this study. Once the participant was equipped, he was asked to walk on two surfaces with inclinations of 5° and 8.4° respectively and data from gyroscope signal and four footswitches were captured through wireless gait detection system.

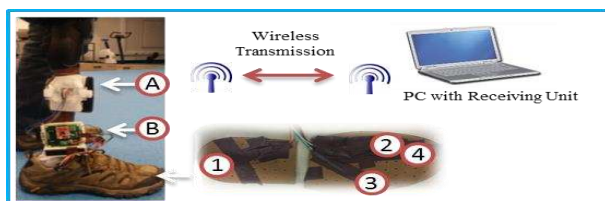


Figure 1. Placement of (A) Gyroscope (B) Base Unit and an insole with footswitches at 1-Heel, 2,3-1st & 5th Metatarsals, 4-Toe

*Research is linked to a large project supported by EPSRC (EP/K020462/1).

H. F. Maqbool, M. A. B. Husman, M. I. Awad, Member, IEEE A. Abouhossein, Member, IEEE, A. A. Dehghani-Sanij: School of Mechanical Engineering, University of Leeds, Leeds, LS2 9JT, UK (e-mail: mnhf@leeds.ac.uk; mnmabh@leeds.ac.uk; m.i.awad@leeds.ac.uk; a.abouhossein@leeds.ac.uk; A.A.Deighani-Sanij@leeds.ac.uk). H. F. Maqbool is on study leave from University of Engineering and Technology Lahore, Pakistan.

Gyroscope signal at shank shows prominent peaks and troughs corresponding to mid-swing (M-Sw), IC and TO. A sample of real-time event detection for prosthetic side during ramp ascending is shown in Fig. 2.

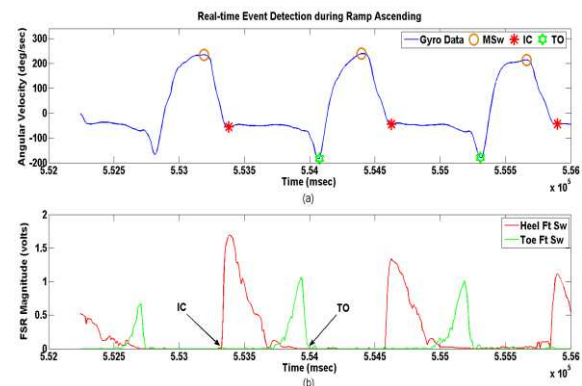


Figure 2. Real-time event detection using (a) gyroscope at shank and validation with (b) footswitches at heel and toe

III. RESULTS

The timing difference was evaluated using; difference = $T_g - T_{fsw}$ where T_g and T_{fsw} indicate the timings of the detected events from gyroscope and footswitches respectively. The mean difference and standard deviation for IC and TO on both inclinations showed quite similar results during ramp ascending for both prosthetic and intact side as shown in Table 1. There are little variations during ramp descending, particularly on prosthetic side. The proposed algorithm showed promising results for both inclined surfaces.

TABLE I. EVENT DETECTION TIME DIFFERENCES (MS) BETWEEN GYROSCOPE AND FOOTSWITCHS: MEAN DIFFERENCE $\pm$ STANDARD DEVIATION

Angle	Ramp Ascending		Ramp Descending	
	5°	8.4°	5°	8.4°
Prosthetic Side				
IC	39 $\pm$ 18	39.5 $\pm$ 20	9 $\pm$ 40	0.7 $\pm$ 5
TO	51 $\pm$ 12	58 $\pm$ 14	23.7 $\pm$ 13	-45.7 $\pm$ 31
Intact Side				
IC	20 $\pm$ 17	28.5 $\pm$ 28	20.3 $\pm$ 26	33.6 $\pm$ 62
TO	21 $\pm$ 9.5	32.3 $\pm$ 24	-3.9 $\pm$ 19	13.5 $\pm$ 15

REFERENCES

- [1] D. Gouwanda and A. A. Gopalai, "A robust real-time gait event detection using wireless gyroscope and its application on normal and altered gait," *Medical Engineering & Physics*, 2015.
- [2] P. Catalfamo, S. Ghousayni, and D. Ewins, "Gait event detection on level ground and incline walking using a rate gyroscope," *Sensors*, vol. 10, pp. 5683-5702, 2010.