



UNIVERSITY OF LEEDS

This is a repository copy of *Spinal angle and foot pressure during cardiac electrophysiological procedures*.

White Rose Research Online URL for this paper:  
<http://eprints.whiterose.ac.uk/81597/>

Version: Accepted Version

---

**Article:**

Ma'touq, J, Strauss, DN, Messenger, N et al. (2 more authors) (2014) Spinal angle and foot pressure during cardiac electrophysiological procedures. *International Journal of Cardiology*, 172 (3). 398 - 400. ISSN 0167-5273

<https://doi.org/10.1016/j.ijcard.2013.12.260>

---

**Reuse**

Unless indicated otherwise, fulltext items are protected by copyright with all rights reserved. The copyright exception in section 29 of the Copyright, Designs and Patents Act 1988 allows the making of a single copy solely for the purpose of non-commercial research or private study within the limits of fair dealing. The publisher or other rights-holder may allow further reproduction and re-use of this version - refer to the White Rose Research Online record for this item. Where records identify the publisher as the copyright holder, users can verify any specific terms of use on the publisher's website.

**Takedown**

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing [eprints@whiterose.ac.uk](mailto:eprints@whiterose.ac.uk) including the URL of the record and the reason for the withdrawal request.



[eprints@whiterose.ac.uk](mailto:eprints@whiterose.ac.uk)  
<https://eprints.whiterose.ac.uk/>

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23

**Spinal angle and foot pressure during cardiac electrophysiological  
procedures**

J. Ma'touq (MSc)<sup>1</sup>, D. N. Straus (PhD)<sup>2</sup>, N. Messenger (PhD)<sup>2</sup>, T. D. Stewart (PhD)<sup>1</sup>, M. H.  
Tayebjee (MD)<sup>3</sup>

<sup>1</sup> Institute of Medical and Biological Engineering, Faculty of Engineering, The University of  
Leeds, UK

<sup>2</sup> Sports and Exercise Sciences, Faculty of Biological Sciences, The University of Leeds,  
UK

<sup>3</sup> West Yorkshire Arrhythmia Service, Department of Cardiology, Leeds General Infirmary,  
UK

Short title : Foot pressure and spinal angle

Word count : 948

Corresponding author:

Dr. Muzahir Tayebjee

Department of Cardiology

Leeds General Infirmary,

Leeds,

24 LS1 3EX

25 United Kingdom

26 [Muzahir.Tayebjee@leedsth.nhs.uk](mailto:Muzahir.Tayebjee@leedsth.nhs.uk)

27 Phone +44 113 3926619 Fax +44 113 3923981

28

29 **Acknowledgment:**

30 The authors have no competing interests. J. Ma'touq was supported by a Said  
31 Foundation Scholarship. This study was also supported by the National Institute for  
32 Health Research (NIHR) through funding of the Leeds Musculoskeletal Biomedical  
33 Research Unit (LMBRU). The Wellcome Trust and EPSRC support WELMEC, a Leeds  
34 Centre of Excellence in Medical Engineering, under grant number WT088908/Z/09/Z.  
35 Ethical approval was obtained by MEEC Faculty Research Ethics Committee, University  
36 of Leeds, Ref:MEEC 11-026

37

38 **Keywords:** Posture, Biomechanics, Foot Pressure, Spine, Cardiac Electrophysiology

39

40 Procedures in interventional cardiology requiring the use of ionising radiation require the  
41 use of lead aprons (6-10kg). In invasive cardiac electrophysiology, procedures may  
42 have a duration of up to 8 hours that results in fatigue, orthopaedic problems (e.g. back  
43 and foot) and impaired venous return [1, 2]. There have been several qualitative (rather  
44 than quantitative) studies investigating the causal link between lead aprons use and  
45 musculoskeletal disorders [2-7].

46 In order to investigate the effects of wearing a lead apron on the spine and feet, a pilot  
47 biomechanical analytical study on a single interventional cardiac electrophysiologist was  
48 conducted.

49

50 One 37 year old male consultant interventional cardiac electrophysiologist performing  
51 invasive cardiac procedures for 10 years with no history of musculoskeletal disorders  
52 was analysed. The subject wore a wrap around lead apron that was not open in the  
53 back. The apron comprised a separate chest jacket and skirt with a belt. Spinal angles  
54 were assessed clinically using video images taken at 30 minute intervals using a  
55 Panasonic HDC-TM900 video camera (Panasonic UK Ltd.). Thoracic and lumbar  
56 angles were measured by manually drawing a tangent for the thoracic and lumbar  
57 segments of the spine. The methodology was initially validated using a 12 camera  
58 Qualisys ProReflex MCU240 motion capture system and C-Motion Visual 3D software  
59 in the Motion Analysis Laboratory where the electrophysiologists operating table and  
60 monitors were simulated. Analysis of 'clinical' spinal angles was completed at regular  
61 time intervals for 5 complete 'live' procedures. Assessment was also conducted in a

62 'laboratory' setting where the clinical procedures were simulated whilst the lead apron  
63 was not being worn.

64 The recording of foot pressure was completed using a Pedar X system (Novel-gmbh) in-  
65 shoe pressure measurement system. The signal was divided into nine zones to aid in  
66 studying changes in the centre of pressure. Filming and foot pressure measurement  
67 were synchronised manually to associate a given task or posture to the foot pressure  
68 measurement. Analysis of foot pressure was completed for 3 complete clinical  
69 procedures with the Pedar equipment calibrated prior to the study and the insoles were  
70 re-set to zero pressure prior to each procedure. Further analysis was also completed on  
71 three resting days (5 different recordings per day to assess variability) when the  
72 electrophysiologist performed no procedures and thus wore no apron as a method of  
73 comparing the clinical results to normal foot pressure.

74 Spinal angles and foot pressures were measured for four different common tasks of the  
75 electrophysiology procedure namely, standing in an upright position, looking at a high  
76 monitor, looking at a low monitor and looking at a side monitor. Results are presented  
77 by comparing the increase in flexion that occurred for each task compared to normal  
78 upright standing.

79

80 When a lead apron was worn the lumbar flexion angle increased by 11°, 23.9, and 4.7°,  
81 compared to upright standing, when looking at the high monitor, looking at the low  
82 monitor and looking at the side monitor, respectively. The corresponding increase in

83 thoracic flexion angles, compared to upright standing, with the lead apron were 11.5°,  
84 25.3°, 1.9° for the same activities respectively.

85 There was no significant difference in flexion angle increase when the  
86 electrophysiologist was analysed in the 'laboratory' when not wearing the apron  
87 (resting) compared to in the 'clinical' setting. Flexion angles were greatest when looking  
88 at the low monitor. Despite looking upwards at the high monitor the electrophysiologist  
89 tended to lean forwards during this activity.

90 Average and peak foot pressure for the three procedures were found to reduce on  
91 resting days and varied with time. Furthermore, high pressure regions were observed  
92 over a significantly greater area of the foot (Figure 1). In addition, as the procedure  
93 progressed the centre of pressure was observed to move towards the anterior aspect of  
94 the foot.

95 Interventional cardiac electrophysiological procedures require multiple changes in  
96 posture, bending and prolonged standing whilst wearing lead aprons. This is to allow a  
97 variety of tasks (including fine motor, and operation of foot pedals) to be completed as  
98 well as to facilitate the observation of multiple monitors often placed sided by side and  
99 above each other.

100

101 Increases in lumbar and thoracic flexion angles up to 25° were observed whilst the 6kg  
102 lead apron was worn and directly associated to the task completed. This finding is  
103 consistent with musculoskeletal adaptations during longer term lead apron wearing [7].

104

105 Foot pressure was shown to be highly variable and dependent upon weight distribution  
106 that shifted regularly during the operation from one leg to both legs. Standing for long  
107 periods of time whilst wearing a lead apron resulted in a 50% increase in both the mean  
108 and maximum peak foot pressures additionally moving the centre of pressure toward  
109 the forefoot region as the procedure progressed and the operator fatigued.

110 The study was conducted on a single operator, however the measurements were  
111 repeated for five procedures. Future work should focus on measuring the effects of  
112 wearing the lead aprons on different operators and at different times of the day.  
113 Equipment used for collecting data in the study was selected specifically as not to  
114 restrict the movement of the operator or influence the clinical environment limiting the  
115 measurement of spinal angles to a simple camera system.

116

117 We show for the first time how musculoskeletal stresses in the cardiac catheter  
118 laboratory can be quantified and provide data to document the effect on the foot and the  
119 spine. Further work is required to confirm these findings, and urgent solutions sought to  
120 seek preventative measures.

121

122 Informed consent was obtained from the electrophysiologist and the study protocol  
123 conforms to the ethical guidelines of the 1975 Declaration of Helsinki. The authors of

124 this manuscript have certified that they comply with the Principles of Ethical Publishing  
125 in the International Journal of Cardiology.

126

127 **Author contributions.**

128 Concept/design: TS, MHT

129 Data analysis/interpretation: JMT, DNS, NM, TS

130 Drafting article: JMT, TS, DNS, NM, MHT

131 Critical revision of article: TS, DNS, NM, MHT

132

133

134

135 **References**

136

137

- 138 1. Fadl, YY, Ellenbogen KA, Grubb RL Jr, Khoo-Summers L, Lindsay BD. A Review  
139 of Spinal Injuries in the Invasive Cardiologist: Part 1. Biomechanics and Pain  
140 Generation. *Pacing Clin Electrophysiol.* 2007. 30:1012-1019.
- 141 2. Goldstein JA, Balter S, Cowley M, Hodgson J, Klein LW. Occupational Hazards  
142 of Interventional Cardiologists: Prevalence of Orthopedic Health Problems in  
143 Contemporary Practice. *Catheter Cardiovasc Interv.* 2004; 63:407–411.
- 144 3. Ross AM, Segal J, Borenstein D, Jenkins E, Cho S. Prevalence of Spinal Disc  
145 Disease Among Interventional Cardiologists. *Am J Cardiol.* 1997;79:68-70.
- 146 4. Pelz, D.M., Low Back Pain, Lead Aprons, and the Angiographer. *AJNR Am J*  
147 *Neuroradiol.* 1999; 21:1364-000.
- 148 5. Klein LW, Miller DL, Balter S, Laskey W, Haines D, Norbash A, Mauro MA, et al.  
149 Occupational Health Hazards in the Interventional Laboratory: Time for a Safer  
150 Environment. *J Vasc Interv Radiol.* 2009; 20:147-152.
- 151 6. Meakin JR, Smith FW, Gilbert FJ, Aspden RM. The effect of axial load on the  
152 sagittal plane curvature of the upright human spine in vivo. *J Biomech.* 2008; 41:  
153 2850-2854.
- 154 7. Johnson DD, Kirkpatrick AE, Ashton-Miller JA, Shih AJ. Effect of Lead Use on  
155 Back and Shoulder Postural Muscle Activity in Healthy Young Adults. *Hum*  
156 *Factors* 2011; 53: 729-739.

157

158

159


160

161 Figure 1. Typical foot pressure results when wearing a lead apron and not wearing a lead apron (rest  
162 day).

163

164

165

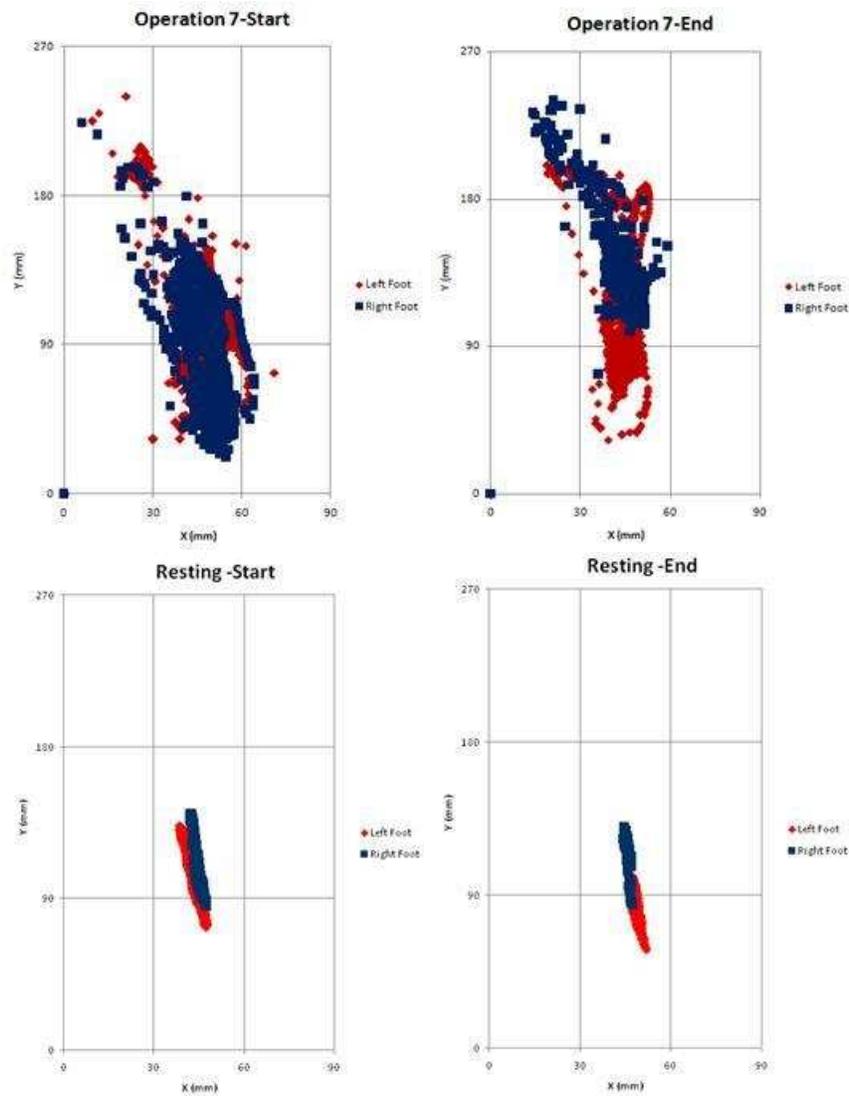

166

167

168

169

170

171