

This is a repository copy of *Cost-effectiveness of implantable cardiac devices in patients with systolic heart failure*.

White Rose Research Online URL for this paper:

<https://eprints.whiterose.ac.uk/100095/>

Version: Accepted Version

---

**Article:**

Mealing, Stuart, Woods, Bethan Sarah orcid.org/0000-0002-7669-9415, Hawkins, Neil et al. (6 more authors) (2016) Cost-effectiveness of implantable cardiac devices in patients with systolic heart failure. *Heart*. ISSN 1468-201X

---

**Reuse**

Items deposited in White Rose Research Online are protected by copyright, with all rights reserved unless indicated otherwise. They may be downloaded and/or printed for private study, or other acts as permitted by national copyright laws. The publisher or other rights holders may allow further reproduction and re-use of the full text version. This is indicated by the licence information on the White Rose Research Online record for the item.

**Takedown**

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing [eprints@whiterose.ac.uk](mailto:eprints@whiterose.ac.uk) including the URL of the record and the reason for the withdrawal request.

# Heart

## Cost-effectiveness of implantable cardiac devices in patients with systolic heart failure

Journal:	<i>Heart</i>
Manuscript ID	heartjnl-2015-308883.R2
Article Type:	Original research article
Date Submitted by the Author:	n/a
Complete List of Authors:	Mealing, Stuart; ICON Health Economics and Epidemiology, Woods, Beth; University of York, Centre for Health Economics; University of York, Centre for Health Economics Hawkins, Neil; London School of Hygiene and Tropical Medicine, Department of Health Services Research and Policy Cowie, Martin; Imperial College London, National Heart & Lung Institute Plummer, Christopher; Freeman Hospital, Department of Cardiology Abraham, William; The Ohio State University, Director, Division of Cardiovascular Medicine Beshai, John Klein, Helmut; University of Rochester Medical Center, Heart Research; Isar Medical center, Cardiology Sculpher, Mark; Oxford Outcomes Ltd., Health Economics; University of York, Centre for Health Economics
Keywords:	Implanted cardiac defibrillators < Electrophysiology < CARDIAC PROCEDURES AND THERAPY, Pacemakers < Electrophysiology < CARDIAC PROCEDURES AND THERAPY, Heart failure with reduced ejection fraction < Heart failure < DISEASES, Health care economics < Health Services < RESEARCH APPROACHES, Micro simulation < Statistics and study design < RESEARCH APPROACHES
Abstract:	<p>Objective To evaluate the cost-effectiveness of implantable cardioverter-defibrillators (ICD), cardiac resynchronisation therapy pacemakers (CRT-P) and combination therapy (CRT-D) in patients with heart failure with reduced ejection fraction based on a range of clinical characteristics.</p> <p>Methods Individual patient data from 13 randomised trials were used to inform a decision analytic model. A series of regression equations were used to predict baseline all-cause mortality, hospitalisation rates and health related quality of life (HRQoL) and device-related treatment effects. Clinical variables used in these equations were age, QRS duration, NYHA class, ischemic aetiology, and LBBB. A UK NHS perspective and a lifetime time horizon were used. Benefits were expressed as quality adjusted life years (QALYs). Results were reported for 24 subgroups based on LBBB status, QRS duration and NYHA class.</p> <p>Results</p>

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

	<p>At a threshold of £30,000 per QALY gained, CRT-D was cost-effective in 10 of the 24 subgroups including all LBBB morphology patients with NYHA I/III/III. ICD is cost-effective for all non-NYHA IV patients with QRS duration &lt;120ms and for NYHA I/II non-LBBB morphology patients with QRS duration between 120 and 149ms. CRT-P was also cost-effective in all NYHA III/IV patients with QRS duration &gt;120ms. Device therapy is cost-effective in most patient groups with LBBB at a threshold of £20,000 per QALY gained. Results were robust to altering key model parameters.</p> <p>Conclusions At a threshold of £30,000 per QALY gained, CRT-D is cost-effective in a far wider group than previously recommended in the UK. In some subgroups ICD and CRT-P remain the cost-effective choice.</p>
--	---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------

SCHOLARONE™  
Manuscripts

Confidential: For Review Only

# Cost-effectiveness of implantable cardiac devices in patients with systolic heart failure

Mealing S<sup>1,\*</sup>, Woods B<sup>2</sup>, Hawkins N<sup>1</sup>, Cowie MR<sup>3</sup>, Plummer CJ<sup>4</sup>, Abraham WT<sup>5</sup>, Beshai JF<sup>6</sup>, Klein H<sup>7</sup>, Sculpher M<sup>1,2</sup>

1) ICON Clinical Research (UK) Ltd. Oxford, UK; 2) Centre for Health Economics, University of York, York, UK; 3) Imperial College London (Royal Brompton Hospital), London, UK; 4) Freeman Hospital, Newcastle upon Tyne, UK; 5) Ohio State University Medical Centre, OH, US  
6) Mayo Clinic, Phoenix, AZ, USA.; 7) University of Rochester, NY, USA

\* Corresponding author (also request for reprints)

Stuart Mealing, Divisional Principal, European Head Health Economics

ICON Clinical Research (UK) Ltd. West Way, Botley

OX2 0JJ, United Kingdom

Tel: +44 (0)1865 324930

Fax: +44 (0)1865 324931

Email: [stuart.mealing@iconplc.com](mailto:stuart.mealing@iconplc.com)

Author	Details
Bethan Woods	Centre for Health Economics, University of York, York, UK
Neil Hawkins	ICON Health Economics, ICON Clinical Research (UK) Ltd. Abingdon, UK
Martin Cowie	Faculty of Medicine, National Heart & Lung Institute ,Imperial College London (Royal Brompton Hospital), London, UK
Chris Plummer	Cardiothoracic Directorate, Freeman Hospital, Newcastle upon Tyne, UK
William Abraham	Department of internal medicine Ohio State University Medical Centre, Ohio, US
John Beshai	Department of cardiovascular diseases Mayo Clinic, Phoenix, AZ, USA
Helmut Klein	University of Rochester medical centre, University of Rochester, NY, USA
Mark Sculpher	Centre for Health Economics, University of York, York, UK

## Abstract (250 words)

### Objective

To evaluate the cost-effectiveness of implantable cardioverter-defibrillators (ICD), cardiac resynchronisation therapy pacemakers (CRT-P) and combination therapy (CRT-D) in patients with heart failure with reduced ejection fraction based on a range of clinical characteristics.

### Methods

Individual patient data from 13 randomised trials were used to inform a decision analytic model. A series of regression equations were used to predict baseline all-cause mortality, hospitalisation rates and health related quality of life and device-related treatment effects. Clinical variables used in these equations were age, QRS duration, NYHA class, ischemic aetiology, and LBBB. A UK NHS perspective and a lifetime time horizon were used. Benefits were expressed as quality adjusted life years (QALYs). Results were reported for 24 subgroups based on LBBB status, QRS duration and NYHA class.

### Results

At a threshold of £30,000 per QALY gained, CRT-D was cost-effective in 10 of the 24 subgroups including all LBBB morphology patients with NYHA I/II/III. ICD is cost-effective for all non-NYHA IV patients with QRS duration <120ms and for NYHA I/II non-LBBB morphology patients with QRS duration between 120 and 149ms. CRT-P was also cost-effective in all NYHA III/IV patients with QRS duration >120ms. Device therapy is cost-effective in most patient groups with LBBB at a threshold of £20,000 per QALY gained. Results were robust to altering key model parameters.

## Conclusions

At a threshold of £30,000 per QALY gained, CRT-D is cost-effective in a far wider group than previously recommended in the UK. In some subgroups ICD and CRT-P remain the cost-effective choice.

## Keywords

*Cardiac Resynchronisation, Implantable Cardioverter Defibrillator, Cost-effectiveness, Cost-utility, CRT, ICD*

## Key questions

### *What is already known about this subject?*

Clinical guidelines on ICD/CRT in HF make recommendations for ICD, CRT-P and CRT-D based on a range of clinical parameters. These include NYHA class, LVEF, ischaemic aetiology status, QRS duration, and presence or absence of either AF or LBBB. ICD and CRT therapy are not indicated in all patient groups of interest.

ICD, CRT-P and CRT-D have been shown to represent a cost-effective use of UK health care expenditure when compared to medical therapy, and when evaluated in patient groups determined by individual trial inclusion criteria.

### *What does this study add?*

We have compared the devices to each other, as well as no device therapy in a much wider set of patients than has previously been evaluated in order to provide an answer to the question 'in which patients are ICD/CRT-P/CRT-D cost-effective?'.

Data from multiple RCTs rather than single studies were used to inform the cost-effectiveness analysis hence results are more reflective of the totality of the clinical data. Results are stratified by a series of commonly used clinical parameters and present health care decision makers with much more information than was previously available.

Device therapy is cost effective at a threshold of £30,000 per QALY gained in all sub-groups examined. CRT-D is cost effective in 10 of the 24 subgroups, and is cost effective for all LBBB morphology patients with NYHA I-III. ICDs are cost effective for all NYHA I-III patients with a QRS duration <120ms and for NYHA I-II patients with non-LBBB morphology and a QRS duration between 120 and 149ms. CRT-P is cost-effective for all NYHA IV patients evaluated.

### *How might this impact on clinical practice?*

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

The results from our work will allow health care decision makers to make more informed decisions on which devices to offer patients taking in to account both clinical and economic factors.

Confidential: For Review Only

## Introduction

In addition to guideline directed medical therapy, implantable cardiac devices have an established role in the treatment of heart failure with reduced ejection fraction (HFrEF). International clinical guidelines<sup>1-3</sup> make recommendations for implantable cardioverter defibrillators (ICD), cardiac resynchronisation therapy pacemakers (CRT-P), and the combined device, CRT-D, based on the presence of specific patient characteristics, recognising that the extent of clinical benefit associated with these devices varies across subgroups within the broader population of patients with HFrEF.

Health care systems internationally are seeking evidence on the value for money of medical interventions, and ICD and CRT have been the subject of a number of economic evaluations<sup>4-9</sup> and health technology assessments (HTAs)<sup>10-12</sup>. In general, the conclusion has been that ICD and CRT are cost-effective when compared to medical therapy, and that CRT-D is marginally cost-effective when compared to standalone CRT-P.

Clinical guidelines on ICD/CRT in HF make recommendations based on a range of clinical parameters. These include New York Heart Association (NYHA) class, Left Ventricular Ejection Fraction (LVEF), ischaemic aetiology status, QRS duration, and presence or absence of either Atrial Fibrillation (AF) or Left Bundle Branch Block (LBBB).<sup>2;3</sup> Guidance issued by HTA organisations such as the National Institute for Health and Care Excellence (NICE)<sup>13;14</sup> is based on a subset of these parameters. The great majority of published ICD/CRT economic evaluations, however, including those informing NICE decisions, have been based on data or populations from single clinical trials. These analyses do not, therefore, reflect the totality of randomised controlled trial evidence available, and have only limited information with which to explore the potential for cost-effectiveness (and decisions based on cost-effectiveness) to vary by patient sub-groups.



1  
2  
3 This paper reports a unique collaboration between manufacturers, clinicians and health  
4  
5 economists to pool individual patient data from all major randomised controlled trials of these  
6  
7 devices (N=12,638). This database of studies has been used to inform a range of research  
8  
9 studies.<sup>15;16</sup> We report its use to develop a cost-effectiveness analysis for submission to NICE  
10  
11 as part of their comprehensive review of ICD and CRT designed to answer the question ‘in  
12  
13 which patients are ICD/CRT-P/CRT-D cost-effective?’.<sup>16</sup> Unlike previous studies, the analysis is  
14  
15 based on a synthesis of evidence across trials and reflects important differences between sub-  
16  
17 groups, hence guiding health systems’ resource allocation decisions regarding these devices.  
18  
19  
20  
21  
22

## 23 **Methods**

### 24 **Decision analytic modelling**

25  
26 The analysis is based on a typical UK HFREF patient population, starting age of 66 years, all  
27  
28 NYHA classes), and LVEF  $\leq 35\%$ . The cost-effectiveness analysis follows the methods  
29  
30 recommended by NICE.<sup>17</sup> Costs considered are those of the UK NHS, and outcomes are  
31  
32 expressed as quality-adjusted life-years (QALYs). An annual discount rate of 3.5% is applied to  
33  
34 both costs and benefits.<sup>17</sup>  
35  
36  
37  
38  
39

40 The analysis is based on a decision analytic model which comprises a series of regression  
41  
42 equations to predict: mortality, hospitalisation rates and health related quality of life (HRQoL).  
43  
44 The regression equations include covariables representing patients’ baseline prognostic  
45  
46 characteristics. The first regression equation predicts the probability of death in patients who  
47  
48 only receive medical therapy. This is combined with estimates of the treatment effects of ICD,  
49  
50 CRT-P and CRT-D based on the results of a network meta-analyses<sup>15</sup> to derive device-specific  
51  
52 mortality probabilities. A second equation is used to predict the monthly probability of  
53  
54 experiencing a hospitalisation event for any reason. A final equation estimates a patient’s  
55  
56 HRQoL given their characteristics and treatment. All living patients potentially incur other costs  
57  
58  
59  
60

1  
2  
3 related to device implant and replacement, background medication and routine clinical visits.  
4

5  
6 Cost-effectiveness results are generated in a two-stage process. In the first stage, costs and  
7  
8 QALYs are estimated for all interventions for all possible sets of patient characteristics ('patient  
9  
10 profiles'). In the second, these are collapsed to 24 subgroups defined by NYHA class, QRS  
11  
12 duration and presence or absence of LBBB. Due to clinical contra-indications or a paucity of  
13  
14 evidence, not all treatments are evaluated for each of the 24 sub-groups (see **supplementary**  
15  
16 **material, Appendix 1**, for details).  
17

18  
19 Expected (mean) costs and QALYs are estimated for all relevant treatments in each sub-group,  
20  
21 and the following standard 'decision rules' are followed to identify the cost-effective intervention  
22  
23 in each sub-group.<sup>18</sup> Firstly, any option that is less effective and more costly than one or more  
24  
25 others is removed from consideration (dominated). Secondly, the extra cost per additional QALY  
26  
27 (the incremental cost effectiveness ratio (ICER)) of a more effective treatment is calculated and  
28  
29 any treatment that is less effective than another with a higher ICER is removed from  
30  
31 consideration (extended dominance). The remaining options lie on a cost-effectiveness 'frontier'  
32  
33 which runs from least to most costly/ effective. ICERs are calculated between each  
34  
35 progressively more costly and effective option.  
36  
37  
38  
39

### 40 **Estimating model inputs**

41  
42 The baseline mortality risk (patients receiving medical therapy alone) was estimated using  
43  
44 relevant individual patient data from the included trials.<sup>15</sup> Parametric survival analysis was used  
45  
46 to extrapolate these mortality risks beyond the follow-up periods in the trials in order to generate  
47  
48 lifetime estimates. The following candidate baseline covariables were selected based on data  
49  
50 availability, a review of risk scores, clinical guidelines, RCT subgroup analyses and clinical  
51  
52 advice: age, QRS duration, LVEF, gender, NYHA class, ischaemic aetiology, LBBB status and a  
53  
54 binary geographic indicator to track whether or not patients were from a North American centre.  
55  
56 Final covariable selection in all regression models was via a stepwise procedure unless  
57  
58  
59  
60

1  
2  
3 otherwise stated. Estimation of the treatment effects of the devices on all-cause mortality has  
4 been detailed elsewhere.<sup>15</sup> Mortality treatment effects were assumed to be maintained for 7.5  
5 years (the maximum follow up period in the trials) after which they would decline so that, by 20  
6 years, there was no impact on mortality.  
7  
8  
9

10  
11  
12 The expected number of all-cause hospitalisations per month for patients on medical therapy,  
13 together with the treatment effects of the devices, was estimated from the 11 trials reporting  
14 relevant data (full list of studies reported in **supplementary material, Appendix 2**).  
15  
16

17  
18 Hospitalisation rates were assumed constant over a patient's lifetime. Excluding LBBB  
19 morphology, the covariates of interest were as for all-cause mortality. NYHA I-II patients were  
20 considered together due to paucity of data on NYHA I patients. For the analysis of the effect of  
21 devices on hospitalisation rates, study specific intercepts were included as well as device  
22 related main effects with interaction terms used to identify treatment effect modifiers.  
23  
24  
25

26  
27 HRQoL estimates expressed on a zero (equivalent of dead) to one (equivalent of good health)  
28 scale are necessary to quality-adjust survival and calculate QALYs.<sup>18</sup> Baseline HRQoL  
29 conditional upon patients' characteristics was estimated using data from the three trials  
30 reporting EQ-5D data (relevant studies listed in **supplementary material, Appendix 2**). The  
31 treatment effects of devices are estimated as the change from baseline (to first follow-up) in the  
32 treatment arms of the included trials, minus the change from baseline in patients allocated to  
33 medical therapy. This HRQoL treatment effect is assumed to be maintained for five years based  
34 on information in the CARE-HF trial,<sup>19</sup> and then to decline to zero by ten years. Throughout the  
35 model, a decline in HRQoL is applied to reflect ageing, estimated using UK general population  
36 data.<sup>20</sup>  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50

51  
52 Hospitalization costs are based on information on hospitalization type from a UK based  
53 population study.<sup>21</sup> The typical HF medications for each NYHA class are estimated based on a  
54 review of the clinical literature and expert opinion. With the exception of those relating to device  
55  
56  
57  
58  
59  
60

1  
2  
3 systems, all costs are taken from national databases.<sup>22-24</sup> The total implant cost for CRT-P is  
4 based on a relevant Healthcare Resource Group (HRG) code. For CRT-D and ICD, no such  
5 codes exist, so cross-manufacturer average selling prices for both systems and leads were  
6 made available by the Association of British Healthcare Industries (ABHI) for the purpose of this  
7 analysis (**supplementary material, Appendix 3**).

8  
9  
10 Device longevity estimates are based on data from the Central Cardiac Audit Database (CCAD).  
11 Parametric survival models are used to model time to first and subsequent device replacements  
12 (**supplementary material, Appendix 3**).

13  
14 A range of sensitivity and scenario analyses are undertaken to quantify the importance of the  
15 key modelling assumptions. Of particular importance is the uncertainty in assumptions regarding  
16 the duration of the mortality and HRQoL treatment effects. Alternative values explored as  
17 sensitivity analyses were: i) a constant, lifetime mortality effect (as in previous UK  
18 reimbursement models<sup>10,12</sup>); ii) a five year time period; and iii) the mean follow up period from  
19 the studies included in the data analyses (2.54 years). A sensitivity analysis was also conducted  
20 using lifetime treatment effect durations for both all-cause mortality and HRQoL (as per previous  
21 UK reimbursement models). Further sensitivity analyses were undertaken including varying key  
22 costs, increasing device longevity, the use of an alternative approach to modelling all-cause  
23 hospitalisation and the use of NYHA class as a modifier of all-cause mortality treatment effect.  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42

### 43 **Software**

44 All mortality related analyses were performed in R ([www.r-project.org](http://www.r-project.org)), with all analysis of  
45 hospitalisation and HRQoL performed in STATA V12 (StataCorp. College Station, TX:  
46 StataCorp LP). The economic model was developed in Microsoft Excel® (Microsoft Corporation,  
47 Redmond, WA).  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

## Results

### All-cause mortality

Full details of the mortality model are reported in the **supplementary material (Appendix 4)**.

The risk of death was higher in patients who are older, male or with ischaemic aetiology. The risk of death was also found to increase across NYHA classes, and was more than three times higher in individuals in NYHA class IV than those in NYHA I/II. The risk of mortality was lower in patients with a normal (<120ms) vs. longer QRS duration (hazard ratio = 0.84) and decreased as LVEF increased. Long term survival predictions for each subgroup and treatment are presented in the **supplementary material (Appendix 5)**. Allowing for variations in within-group sample size and covariate mix the results are broadly internally consistent and in line with the published literature.

### All cause hospitalisation

Full details of the baseline hospitalisation model are reported in the **supplementary material (Appendix 4)**. Patients in NYHA classes III and IV were 2.1 and 4.4 times, respectively, more likely to be hospitalised than those in NYHA I/II. Ischaemic aetiology increased the rate of hospitalisation by 9% and wide QRS complex increased the rate by 22% (120-149ms) and 6% (150ms or more), respectively.

The model predicted that ICDs reduced monthly hospitalisation rates by 20% in patients with NYHA I/II/III HF. CRT-P was associated with reductions in monthly hospitalisation rates of 32% and 40%, respectively, in patients with NYHA III/IV HF. CRT-D was associated with a monthly rate reduction of 30% in patients with NYHA I-IV HF. In NYHA III/IV patients the treatment effects arising from the patient level data for CRT-D compared to those generated for CRT-P were considered clinically implausible. For the base case analysis of these patients we therefore assumed equivalence of efficacy for CRT-D and CRT-P. Subgroup/ treatment specific lifetime

1  
2  
3 hospitalisation counts are reported in **supplementary material (Appendix 5)**. These data  
4  
5 require careful interpretation since subgroups with longer overall survival have more  
6  
7 hospitalisation events.  
8  
9

### 10 **Health related quality of life**

11  
12 Full details of the HRQoL model are reported in the **supplementary material (Appendix 4)**.  
13  
14 Statistically significant ( $p < 0.05$ ) but modest improvements from baseline were observed for ICD  
15  
16 and CRT-D in patients with NYHA I or II heart failure, and CRT-P in NYHA Class III (+0.02,  
17  
18 +0.03 and +0.091, respectively). No significant impact was observed on HRQoL with ICD or  
19  
20 CRT-D therapy in patients in NYHA Class III. Meaningful results for patients with NYHA IV HF  
21  
22 could not be generated due to the very low numbers of patients in the clinical trials.  
23  
24  
25

26  
27 For the purposes of economic modelling, equivalence of HRQoL benefit for CRT-P and CRT-D  
28  
29 was again assumed in NYHA III and IV HF. This assumption can be justified on the basis of a  
30  
31 review of external sources and trial specific Minnesota Living with Heart Failure data.<sup>16</sup>  
32  
33

### 34 **Cost effectiveness – base case**

35  
36 The base case results for all subgroups are presented in **Table 1**. For each patient sub-group,  
37  
38 the order of treatments on the cost-effectiveness frontier is shown, and the ICERs for each  
39  
40 option which is not subject to dominance or extended dominance. **Table 2** shows the cost-  
41  
42 effective option for each sub-group (cost-effectiveness threshold: £30,000 per QALY gained).  
43  
44 Device therapy is cost effective at this threshold in all sub-groups examined. CRT-D is cost  
45  
46 effective in 10 of the 24 subgroups, and is cost effective for all LBBB morphology patients with  
47  
48 NYHA I/II/III. ICDs are cost effective for all non-NYHA IV patients with a QRS duration  $< 120$ ms  
49  
50 and for NYHA I/II, non-LBBB morphology patients with a QRS duration between 120 and  
51  
52 149ms. CRT-P is cost-effective for all NYHA IV patients evaluated.  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3 Results generated using a more stringent threshold value (£20,000 per QALY gained) are  
4 presented in **Table 3**. CRT-D is only cost-effective in two patient groups (NYHA I or II, QRS  
5 duration  $\geq 150$ ms, with LBBB); ICD is only cost-effective in two patient groups (NYHA I or II,  
6 QRS duration between 120 and 149ms, no LBBB); and CRT-P is cost-effective in six patient  
7 groups (NYHA III or IV, QRS duration  $> 120$ ms, and LBBB and also NYHA III/IV, QRS duration  
8  $\geq 150$ ms and no LBBB).  
9  
10  
11  
12  
13  
14  
15

16  
17 The nature of the cost-effective intervention is dependent upon the cost effectiveness threshold  
18 (**Figure 1**). Beyond a threshold value of approximately £24,500 per QALY gained, for patients  
19 without LBBB morphology the treatments identified in the base case analysis are largely robust  
20 to changes in threshold. For patients with LBBB morphology there is generally less sensitivity to  
21 changes in threshold. For patients with LBBB morphology there is generally less sensitivity to  
22 changes in threshold, with the cost-effective treatments presented in **Table 2** largely unchanged  
23 beyond a threshold value of approximately £22,000 per QALY.  
24  
25  
26  
27  
28  
29

30 Results in NYHA I and IV patients are subject to additional uncertainty due to the numbers of  
31 patients informing these analyses and the nature of the trial inclusion criteria for NYHA I  
32 patients, these issues are described in the discussion.  
33  
34  
35  
36  
37

### 38 **Sensitivity analyses**

39  
40 The choice of cost-effective therapy was, in general, unchanged when varying the duration of  
41 maximum all-cause mortality treatment effect (**Table 4**, threshold value £30,000 per QALY  
42 gained). A similar outcome was noted when the assumption of lifetime treatment effect  
43 durations for both all-cause mortality and HRQoL improvements was made (**Table 4**). A detailed  
44 breakdown of the fully incremental ICERs generated in this latter analysis is presented in the  
45 **supplementary material (Appendix 6)**. The corresponding results generated using a threshold  
46 value of £20,000 per QALY gained are presented in **Table 5**.  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3 The impact of varying key costs, increasing device longevity, the use of an alternative approach  
4 to modelling all-cause hospitalisation and the use of NYHA class as an all-cause mortality  
5 treatment effect modifier on the choice of devices at thresholds of £20,000 and £30,000 per  
6 QALY gained was modest. Hence, the model was robust to changes in these parameters.  
7  
8  
9  
10  
11

## 12 13 14 **Discussion**

15  
16  
17 The clinical efficacy of CRT and ICD therapy has been investigated in numerous studies, and  
18 these technologies are established therapies for HFrEF individuals in international practice. The  
19 uniqueness of the database created for the purpose of this analysis lies in the ability to explore  
20 the clinical efficacy of CRT and ICD in detail, and in particular to pursue a thorough investigation  
21 of the impact of key clinical variables on both the baseline risk of death and the efficacy of each  
22 treatment option in reducing mortality.<sup>15</sup> The database also facilitated the incorporation of  
23 clinical sub-groups into the cost-effectiveness assessment so the devices representing best  
24 value for money for patients with different sets of clinical characteristics could be identified.  
25  
26  
27

28  
29  
30 This collaboration can serve as a model for similar collaboration across manufacturers. Pooling  
31 together clinical data across manufactures can help manufactures, physicians, and policy  
32 makers become more confident in the clinical- and cost-effectiveness of a therapy and get a  
33 better understanding of how this varies across patients.  
34  
35  
36

37  
38  
39 The analysis presented here was used to inform the recent NICE guidance regarding the use of  
40 these technologies. The committee developing the NICE recommendations recognized this  
41 analysis as “a rich and important data source”<sup>25</sup>, and based its decision making on it. The  
42 guidance issued by NICE in 2014 reflected the findings of this cost-effectiveness analysis in  
43 almost all subgroups,<sup>25</sup> with the exception of CRT-D in patients with NYHA III and QRS 120-  
44 149ms without LBBB morphology and CRT-D in asymptomatic (NYHA Class I) patients with  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60



1  
2  
3 QRS 120-149ms. ICD was recommended in both cases due to concerns about reduced  
4 effectiveness and a lack of symptomatic benefit of CRT in these subgroups.  
5  
6

7  
8 The major source of uncertainty identified during the NICE appraisal of these technologies was  
9 the duration of treatment effect on all-cause mortality. The duration of effect used in this  
10 analysis (7.5 years) is supported by a number of long-term studies. Recently published data  
11 from the CARE-HF study<sup>19</sup> found that, at a mean follow-up of 56 months in the CRT-P and 50  
12 months in the medical therapy arms, the hazard ratio for all cause-mortality (CRT-P vs. OPT)  
13 was 0.77 [95% CI 0.63, 0.93], despite 39% of control patients crossing-over to a CRT device  
14 during follow-up. In addition, long-term follow-up from the MADIT-II study<sup>26</sup> found that, at a  
15 median follow-up of 7.6 years, the hazard ratio for all cause-mortality (ICD vs. non-ICD) was  
16 0.77 [0.65, 0.91], although 34% of control patients crossed-over to a device during follow-up.  
17 Attempts to adjust statistically for cross-over resulted in treatment effect estimates of 0.67 [0.56,  
18 0.80] and 0.66 [0.56, 0.78], in CARE-HF and MADIT-II, respectively.<sup>19,26</sup>  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31

32 The results from our analysis, generated using a cost-effectiveness threshold of £30,000 per  
33 QALY gained broadly agrees with guidelines issued by the European Society of Cardiology.<sup>3,27</sup>  
34  
35 In patients with QRS<120ms, NYHA II-III and EF≤35%, ICD is recommended and cost-effective  
36 according to our analysis. In ambulatory NYHA IV patients with prolonged QRS duration, CRT-P  
37 is recommended and cost-effective. Our analysis provides information on where scarce  
38 resources should be targeted in patients with QRS prolongation and in NYHA class II or III  
39 where several possible device options are recommended. In particular, it suggests that CRT-D  
40 is cost-effective in NYHA II-III patients with LBBB morphology, and that, in patients with non-  
41 LBBB morphology, CRT-D is cost-effective in all groups with the exception of NYHA II patients  
42 with a QRS duration of 120-149ms. Unlike previous guidelines, the current analysis suggests  
43 implantable devices may be cost-effective in asymptomatic patients (NYHA Class I). However,  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

1  
2  
3 given the small number of patients in these groups in the trials, results in NYHA Class I, and in  
4 particular in relation to CRT-D in this patient group, should be regarded with caution.<sup>15</sup>  
5  
6

7  
8 Comparison of the results from the current analysis with previous UK HTA models of ICD and  
9 CRT is challenging due to the different model structures and evidence used. The earlier models  
10 used aggregate level evidence, whereas the current model was based on access to a large  
11 amount of individual patient data. Accepting these differences, the results from the sensitivity  
12 analysis performed with the removal of all tapering effects on treatment effect durations are the  
13 most comparable with earlier models. This showed that the ICERs from the current analysis are  
14 lower (i.e. better value for money) than those considered acceptable in previous NICE guidance.  
15  
16 The reasons for this are likely to be increases in average device longevity and a reduction in  
17 hardware acquisition costs. In many cases, where ICD was historically recommended, the  
18 current analysis suggests patients should be offered a CRT-D device as the most clinically and  
19 cost-effective option.  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31

32 A number of limitations arose from the choice of modeling approach and data on which the  
33 analyses were based, with the main area of potential concern being that some of the patient  
34 groups modeled were sparsely represented in our database. The primary groups of concern  
35 relate to patients in NYHA Class I and IV HF (regardless of LBBB status). Cost-effectiveness  
36 results in these groups may have been influenced by the small patient numbers and should be  
37 treated with caution. In addition, NYHA I patients in trials may be atypical of those observed in  
38 clinical practice as specific inclusion criteria were used to focus on patients who were easily  
39 identifiable.<sup>28,29</sup>  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49

50 Omitting previous HF hospitalisations as a predictor of subsequent monthly hospitalisation  
51 events represents a limitation of our analysis. However, the total event rates predicted are low  
52 and the choice of modelling approach is therefore unlikely to have had a substantive impact on  
53 the model results.  
54  
55  
56  
57  
58  
59  
60

1  
2  
3 In conclusion, from a UK NHS perspective, at a threshold of £30,000 per QALY gained our  
4  
5 analysis has shown that CRT-D is cost effective in a far wider group of patients than previously  
6  
7 recommended and that, for most other patients, ICD is a cost-effective treatment alternative.  
8  
9 Our analysis also showed that CRT-P was cost-effective in all patients with NYHA III/IV and a  
10  
11 QRS duration >120ms. Device therapy is cost-effective in most patient groups with LBBB at a  
12  
13 threshold of £20,000 per QALY gained.  
14  
15  
16  
17

### 18 **Acknowledgements and affiliations**

19  
20 We would like to acknowledge Dr. David Cunningham (on behalf of CCAD) for making the  
21  
22 device longevity data available (**Supplementary material, Appendix 3**) and to the device  
23  
24 manufacturers for making available all relevant trial data. MRC's salary is supported by the  
25  
26 National Institute for Health Research Cardiovascular Biomedical Research Unit at the Royal  
27  
28 Brompton Hospital, London.  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

## References

1. Hunt SA, Abraham WT, Chin MH, et al. ACC/AHA 2005 Guideline Update for the Diagnosis and Management of Chronic Heart Failure in the Adult: a report of the American College of Cardiology/American Heart Association Task Force on Practice Guidelines (Writing Committee to Update the 2001 Guidelines for the Evaluation and Management of Heart Failure): developed in collaboration with the American College of Chest Physicians and the International Society for Heart and Lung Transplantation: endorsed by the Heart Rhythm Society. *Circulation* 2005;112(12):e154-235.
2. Jessup M, Abraham WT, Casey DE, et al. 2009 focused update: ACCF/AHA Guidelines for the Diagnosis and Management of Heart Failure in Adults: a report of the American College of Cardiology Foundation/American Heart Association Task Force on Practice Guidelines: developed in collaboration with the International Society for Heart and Lung Transplantation. *Circulation* 2009;119(14):1977-2016.
3. McMurray JJ, Adamopoulos S, Anker SD, et al. ESC guidelines for the diagnosis and treatment of acute and chronic heart failure 2012: The Task Force for the Diagnosis and Treatment of Acute and Chronic Heart Failure 2012 of the European Society of Cardiology. Developed in collaboration with the Heart Failure Association (HFA) of the ESC. *Eur J Heart Fail* 2012;14(8):803-69.
4. Noyes K, Veazie P, Hall WJ, et al. Cost-effectiveness of cardiac resynchronization therapy in the MADIT-CRT trial. *J Cardiovasc Electrophysiol* 2013;24(1):66-74.
5. Linde C, Mealing S, Hawkins N, et al. Cost-effectiveness of cardiac resynchronization therapy in patients with asymptomatic to mild heart failure: insights from the European cohort of the REVERSE (Resynchronization Reverses remodeling in Systolic Left Ventricular Dysfunction). *Eur Heart J* 2011;32(13):1631-9.
6. Mark DB, Nelson CL, Anstrom KJ, et al. Cost-effectiveness of defibrillator therapy or amiodarone in chronic stable heart failure: results from the Sudden Cardiac Death in Heart Failure Trial (SCD-HeFT). *Circulation* 2006;114(2):135-42.
7. Al-Khatib SM, Anstrom KJ, Eisenstein EL, et al. Clinical and economic implications of the Multicenter Automatic Defibrillator Implantation Trial-II. *Ann Intern Med* 2005;142(8):593-600.
8. Calvert MJ, Freemantle N, Yao G, et al. Cost-effectiveness of cardiac resynchronization therapy: results from the CARE-HF trial. *Eur Heart J* 2005;26(24):2681-8.
9. Feldman AM, de Lissovoy G, Bristow MR, et al. Cost effectiveness of cardiac resynchronization therapy in the Comparison of Medical Therapy, Pacing, and Defibrillation in Heart Failure (COMPANION) trial. *J Am Coll Cardiol* 2005;46(12):2311-21.
10. Fox M, Mealing S, Anderson R, et al. The clinical effectiveness and cost-effectiveness of cardiac resynchronisation (biventricular pacing) for heart failure: systematic review and economic model. *Health Technol Assess* 2007;11(47):iii-iv, ix-248.

- 1  
2  
3 11. Medical Services Advisory Committee Australian Government Department of Health and Aging.  
4 Cardiac resynchronisation therapy for severe heart failure. 2006.  
5
- 6  
7 12. Buxton M, Caine N, Chase D, et al. A review of the evidence on the effects and costs of implantable  
8 cardioverter defibrillator therapy in different patient groups, and modelling of cost-effectiveness  
9 and cost-utility for these groups in a UK context. *Health Technol Assess* 2006;10(27):iii-iv, ix-xi,  
10 1-164.  
11
- 12 13. National Institute for Health and Clinical Excellence. Implantable Cardioverter Defibrillators for  
13 Arrhythmias: Final Appraisal Determination.  
14 [http://www.nice.org.uk/nicemedia/pdf/Arrhythmias\\_FAD.pdf](http://www.nice.org.uk/nicemedia/pdf/Arrhythmias_FAD.pdf)  
15
- 16 14. National Institute for Health and Clinical Excellence. Cardiac resynchronisation therapy for the  
17 treatment of heart failure: Final Appraisal Determination.  
18 [http://www.nice.org.uk/nicemedia/pdf/Heartfailure\\_FAD.pdf](http://www.nice.org.uk/nicemedia/pdf/Heartfailure_FAD.pdf)  
19
- 20 15. Woods B, Hawkins N, Mealing S, et al. Individual patient data network meta-analysis of mortality  
21 effects of implantable cardiac devices. *Heart* 2015;101(22):1800-6.  
22
- 23 16. Association of British Healthcare Industries. Implantable cardioverter defibrillators for the treatment  
24 of arrhythmias and cardiac resynchronisation therapy for the treatment of heard failure (review  
25 of TA95 and TA120): Submission to the National Institute for Health and Care Excellence.  
26 <https://www.nice.org.uk/guidance/ta314/documents>.  
27
- 28 17. National Institute for Health and Care Excellence. Guide to the Methods of Technology Appraisal.  
29 <https://www.nice.org.uk/article/pmg9/chapter/foreword>  
30
- 31 18. Briggs A CK, Sculpher M. Decision Modelling for Health Economic Evaluation. Oxford University Press;  
32 2006.  
33
- 34 19. Cleland JG, Freemantle N, Erdmann E, et al. Long-term mortality with cardiac resynchronization  
35 therapy in the Cardiac Resynchronization-Heart Failure (CARE-HF) trial. *Eur J Heart Fail*  
36 2012;14(6):628-34.  
37
- 38 20. Kind P HG, Macran S. . UK Population Norms for EQ-5D.  
39 [https://www.york.ac.uk/media/che/documents/papers/discussionpapers/CHE%20Discussion%20](https://www.york.ac.uk/media/che/documents/papers/discussionpapers/CHE%20Discussion%20Paper%20172.pdf)  
40 [Paper%20172.pdf](https://www.york.ac.uk/media/che/documents/papers/discussionpapers/CHE%20Discussion%20Paper%20172.pdf)  
41
- 42 21. Cowie MR, Fox KF, Wood DA, et al. Hospitalization of patients with heart failure: a population-based  
43 study. *Eur Heart J* 2002;23(11):877-85.  
44
- 45 22. Department of Health. NHS Reference costs 2012. [https://www.gov.uk/government/collections/nhs-](https://www.gov.uk/government/collections/nhs-reference-costs)  
46 [reference-costs](https://www.gov.uk/government/collections/nhs-reference-costs)  
47
- 48 23. Curtis L. Unit costs of health and social care 2012 <http://www.pssru.ac.uk/>  
49
- 50 24. British National Formulary. <http://www.bnf.org/>  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

- 1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60
25. National Institute for Health and Care Excellence. Implantable cardioverter defibrillators and cardiac resynchronisation therapy for arrhythmias and heart failure (review of TA95 and TA120): <http://www.nice.org.uk/guidance/ta314/documents/arrhythmias-icds-heart-failure-cardiac-resynchronisation-fad-document2>.
  26. Goldenberg I, Gillespie J, Moss AJ, et al. Long-term benefit of primary prevention with an implantable cardioverter-defibrillator: an extended 8-year follow-up study of the Multicenter Automatic Defibrillator Implantation Trial II. *Circulation* 2010;122(13):1265-71.
  27. The Task Force on Cardiac Pacing Resynchronization Therapy of the European Society of Cardiology. Developed in collaboration with the European Heart Rhythm A, Brignole M, Auricchio A, et al. 2013 ESC Guidelines on cardiac pacing and cardiac resynchronization therapy. *Rev Esp Cardiol (Engl Ed)* 2014;67(1):58.
  28. Linde C, Abraham WT, Gold MR, et al. Randomized trial of cardiac resynchronization in mildly symptomatic heart failure patients and in asymptomatic patients with left ventricular dysfunction and previous heart failure symptoms. *J Am Coll Cardiol* 2008;52(23):1834-43.
  29. Moss AJ, Hall WJ, Cannom DS, et al. Cardiac-resynchronization therapy for the prevention of heart-failure events. *N Engl J Med* 2009;361(14):1329-38.

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

### Figure legends

Figure 1: Graphic display of cost-effective option across cost-effectiveness threshold values (base case)

Confidential: For Review Only

## Text tables

Table 1: Base case results. Cost-effectiveness sequence relates to the order in which interventions appear on the cost-effectiveness frontier. "N/A" represents fewer than four interventions being considered. Options labelled as "Dominated" or "Ext Dominated" do not lie on the frontier

Patient group	Cost-effectiveness sequence				Incremental cost-effective ratios			
	1 <sup>st</sup>	2 <sup>nd</sup>	3 <sup>rd</sup>	4 <sup>th</sup>	1 <sup>st</sup>	2 <sup>nd</sup>	3 <sup>rd</sup>	4 <sup>th</sup>
<i>Individuals without LBBB morphology</i>								
NYHA I, QRS duration <120ms <sup>a</sup>	MT	ICD	N/A	N/A	Referent	£24,074	N/A	N/A
NYHA I, QRS duration ≥120ms and <150ms <sup>a</sup>	MT	CRT-D	ICD	N/A	Referent	Dominated	£16,253	N/A
NYHA I, QRS duration ≥150ms <sup>a</sup>	MT	ICD	CRT-D	N/A	Referent	£21,102	£21,759	N/A
NYHA II, QRS duration <120ms	MT	ICD	N/A	N/A	Referent	£24,465	N/A	N/A
NYHA II, QRS duration ≥120ms and <150ms	MT	CRT-D	ICD	N/A	Referent	Dominated	£16,813	N/A
NYHA II, QRS duration ≥150ms	MT	ICD	CRT-D	N/A	Referent	£20,602	£23,738	N/A
NYHA III, QRS duration <120ms	MT	ICD	N/A	N/A	Referent	£27,826	N/A	N/A
NYHA III, QRS duration ≥120ms and <150ms	MT	CRT-P	ICD	CRT-D	Referent	£20,178	Ext Dominated	£23,349
NYHA III, QRS duration ≥150ms	MT	ICD	CRT-P	CRT-D	Referent	Dominated	£13,930	£25,200
NYHA IV, QRS duration <120ms	MT	N/A	N/A	N/A	Referent	N/A	N/A	N/A
NYHA IV, QRS duration ≥120ms and <150ms	MT	CRT-P	CRT-D	N/A	Referent	£22,578	£40,052	N/A
NYHA IV, QRS duration ≥150ms	MT	CRT-P	CRT-D	N/A	Referent	£17,175	£35,811	N/A
<i>Individuals with LBBB morphology</i>								
NYHA I, QRS duration ≥120ms and <150ms <sup>a</sup>	MT	ICD	CRT-D	N/A	Referent	£20,677	£21,672	N/A
NYHA I, QRS duration ≥150ms <sup>a</sup>	MT	ICD	CRT-D	N/A	Referent	Ext Dominated	£17,470	N/A
NYHA II, QRS duration ≥120ms and <150ms	MT	ICD	CRT-D	N/A	Referent	Ext Dominated	£20,704	N/A
NYHA II, QRS duration ≥150ms	MT	ICD	CRT-D	N/A	Referent	Ext Dominated	£17,664	N/A
NYHA III, QRS duration ≥120ms and <150ms	MT	ICD	CRT-P	CRT-D	Referent	Dominated	£14,215	£24,875



1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49

NYHA III, QRS duration≥150ms	MT	ICD	CRT-P	CRT-D	Referent	Dominated	£10,496	£28,646
NYHA IV, QRS duration≥120ms and <150ms	MT	CRT-P	CRT-D	N/A	Referent	£18,664	£37,104	N/A
NYHA IV, QRS duration≥150ms	MT	CRT-P	CRT-D	N/A	Referent	£14,500	£40,449	N/A

MT: Medical therapy; ICD: Implantable cardioverter-defibrillator; CRTP: standalone CRT device; CRTD: combined CRT and ICD device; N/A: Not applicable; a) Results in NYHA I and IV patients are based on relatively low patient numbers and may be subject to bias due to the nature of trial inclusion criteria for NYHA I patients. For further detail see main text.

Confidential: For Review Only

Table 2: Summary of cost-effectiveness recommendations arising from the base case analysis  
(threshold value: £30,000 per QALY gained)

NYHA	QRS duration<120ms	QRS duration 120-150ms	QRS duration>150ms
<i>Patients without LBBB morphology</i>			
I <sup>a</sup>	ICD	ICD	CRT-D
II	ICD	ICD	CRT-D
III	ICD	CRT-P / CRT-D <sup>b</sup>	CRT-P / CRT-D <sup>b</sup>
IV	Medical therapy	CRT-P	CRT-P
<i>Patients with LBBB morphology</i>			
I <sup>a</sup>		CRT-D	CRT-D
II		CRT-D	CRT-D
III		CRT-P / CRT-D <sup>b</sup>	CRT-P / CRT-D <sup>b</sup>
IV		CRT-P	CRT-P

a) Results in NYHA I and IV patients are based on relatively low patient numbers and may be subject to bias due to the nature of trial inclusion criteria for NYHA I patients. For further detail see main text. b) Instances where NICE recommended two devices based on fully incremental results and a threshold of £30,000 per QALY gained. CRT-P values are relative to medical therapy and CRT-D values relative to CRT-P.

Table 3: Summary of cost-effectiveness recommendations arising from the base case analysis  
(threshold value: £20,000 per QALY gained)

NYHA	QRS duration<120ms	QRS duration 120-150ms	QRS duration>150ms
<i>Patients without LBBB morphology</i>			
I <sup>a</sup>	Medical Therapy	ICD	Medical Therapy
I	Medical Therapy	ICD	Medical Therapy
III	Medical Therapy	Medical Therapy	CRT-P
IV	Medical Therapy	Medical Therapy	CRT-P
<i>Patients with LBBB morphology</i>			
I <sup>a</sup>		Medical Therapy	CRT-D
II		Medical Therapy	CRT-D
III		CRT-P	CRT-P
IV		CRT-P	CRT-P

a) Results in NYHA I and IV patients are based on relatively low patient numbers and may be subject to bias due to the nature of trial inclusion criteria for NYHA I patients. For further detail see main text.

Table 4: Impact of duration of treatment effect on treatment choice (threshold £30,000 per QALY gained). Changes from base case highlighted in bold

Subgroup	Duration of mortality treatment effect				Lifetime mortality and constant HRQoL
	Lifetime	7.5 years	5 years	Mean f/up	
<i>Individuals without LBBB</i>					
NYHA I, QRS <120ms <sup>a</sup>	ICD	ICD	ICD	ICD	ICD
NYHA I, QRS ≥120ms and <150ms <sup>a</sup>	ICD	ICD	ICD	ICD	ICD
NYHA I, QRS ≥150ms <sup>a</sup>	CRT-D	CRT-D	CRT-D	CRT-D	CRT-D
NYHA II, QRS <120ms	ICD	ICD	ICD	ICD	ICD
NYHA II, QRS ≥120ms and <150ms	ICD	ICD	ICD	ICD	ICD
NYHA II, QRS ≥150ms	CRT-D	CRT-D	CRT-D	CRT-D	CRT-D
NYHA III, QRS <120ms	ICD	ICD	ICD	<b>MT</b>	ICD
NYHA III, QRS ≥120ms and <150ms	CRT-D	CRT-D	CRT-D	CRT-D	CRT-D
NYHA III, QRS ≥150ms	CRT-D	CRT-D	CRT-D	CRT-D	CRT-D
NYHA IV, QRS <120ms	MT	MT	MT	MT	MT
NYHA IV, QRS ≥120ms and <150ms	CRT-P	CRT-P	CRT-P	CRT-P	CRT-P
NYHA IV, QRS ≥150ms	CRT-P	CRT-P	CRT-P	CRT-P	CRT-P
<i>Individuals with LBBB</i>					
NYHA I, QRS ≥120ms and <150ms <sup>a</sup>	CRT-D	CRT-D	CRT-D	CRT-D	CRT-D
NYHA I, QRS ≥150ms <sup>a</sup>	CRT-D	CRT-D	CRT-D	CRT-D	CRT-D
NYHA II, QRS ≥120ms and <150ms	CRT-D	CRT-D	CRT-D	CRT-D	CRT-D
NYHA II, QRS ≥150ms	CRT-D	CRT-D	CRT-D	CRT-D	CRT-D
NYHA III, QRS ≥120ms and <150ms	CRT-D	CRT-D	CRT-D	CRT-D	CRT-D
NYHA III, QRS ≥150ms	CRT-D	CRT-D	<b>CRT-P</b>	<b>CRT-P</b>	CRT-D
NYHA IV, QRS ≥120ms and <150ms	CRT-P	CRT-P	CRT-P	CRT-P	CRT-P
NYHA IV, QRS ≥150ms	CRT-P	CRT-P	CRT-P	CRT-P	CRT-P

MT: Medical Therapy; a) Results in NYHA I and IV patients are based on relatively low patient numbers and may be subject to bias due to the nature of trial inclusion criteria for NYHA I patients. For further detail see main text.


Table 5: Impact of duration of treatment effect on treatment choice (threshold £20,000 per QALY gained). Changes from base case highlighted in bold

Subgroup	Duration of mortality treatment effect				Lifetime mortality and constant HRQoL
	Lifetime	7.5 years	5 years	Mean f/up	
<i>Individuals without LBBB</i>					
NYHA I, QRS <120ms <sup>a</sup>	ICD	<b>MT</b>	<b>MT</b>	<b>MT</b>	ICD
NYHA I, QRS ≥120ms and <150ms <sup>a</sup>	ICD	ICD	ICD	ICD	ICD
NYHA I, QRS ≥150ms <sup>a</sup>	CRT-D	<b>MT</b>	<b>MT</b>	<b>MT</b>	CRT-D
NYHA II, QRS <120ms	ICD	<b>MT</b>	<b>MT</b>	<b>MT</b>	ICD
NYHA II, QRS ≥120ms and <150ms	ICD	ICD	ICD	ICD	ICD
NYHA II, QRS ≥150ms	CRT-D	<b>MT</b>	<b>MT</b>	<b>MT</b>	<b>ICD</b>
NYHA III, QRS <120ms	MT	MT	MT	MT	MT
NYHA III, QRS ≥120ms and <150ms	CRT-P	<b>MT</b>	<b>MT</b>	<b>MT</b>	CRT-P
NYHA III, QRS ≥150ms	CRT-P	CRT-P	CRT-P	CRT-P	CRT-P
NYHA IV, QRS <120ms	MT	MT	MT	MT	MT
NYHA IV, QRS ≥120ms and <150ms	MT	MT	MT	MT	MT
NYHA IV, QRS ≥150ms	CRT-P	CRT-P	CRT-P	CRT-P	CRT-P
<i>Individuals with LBBB</i>					
NYHA I, QRS ≥120ms and <150ms <sup>a</sup>	CRT-D	<b>MT</b>	<b>MT</b>	<b>MT</b>	CRT-D
NYHA I, QRS ≥150ms <sup>a</sup>	CRT-D	CRT-D	CRT-D	<b>MT</b>	CRT-D
NYHA II, QRS ≥120ms and <150ms	CRT-D	<b>MT</b>	<b>MT</b>	<b>MT</b>	CRT-D
NYHA II, QRS ≥150ms	CRT-D	CRT-D	CRT-D	<b>MT</b>	CRT-D
NYHA III, QRS ≥120ms and <150ms	CRT-P	CRT-P	CRT-P	CRT-P	CRT-P
NYHA III, QRS ≥150ms	CRT-P	CRT-P	CRT-P	CRT-P	CRT-P
NYHA IV, QRS ≥120ms and <150ms	CRT-P	CRT-P	CRT-P	CRT-P	CRT-P
NYHA IV, QRS ≥150ms	CRT-P	CRT-P	CRT-P	CRT-P	CRT-P

a) Results in NYHA I and IV patients are based on relatively low patient numbers and may be subject to bias due to the nature of trial inclusion criteria for NYHA I patients. For further detail see main text.

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

Figure 1

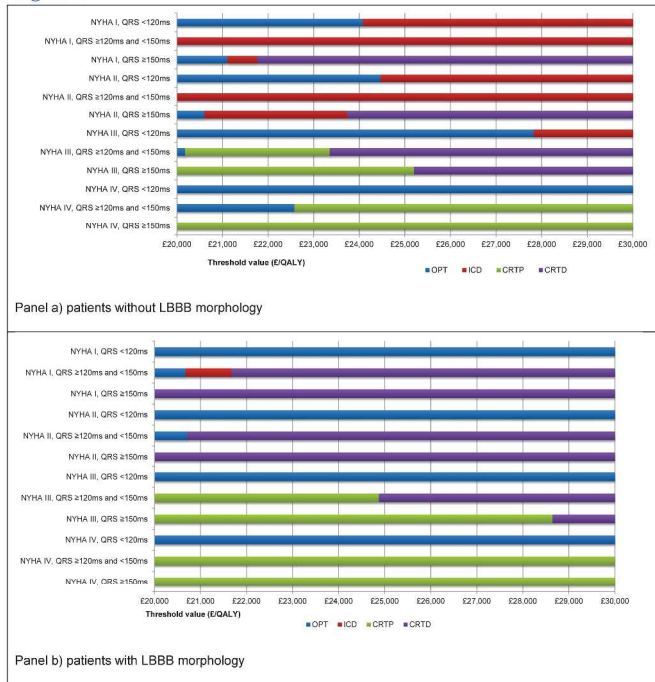

1

Figure 1: Graphic display of cost-effective option across cost-effectiveness threshold values (base case) 297x420mm (300 x 300 DPI)

only

## SUPPLEMENTARY ONLINE MATERIAL

### Appendix 1: Rational for excluding interventions from some subgroups

Table S1: Rationale for excluding interventions from some subgroups

Treatment option	Subgroup from which excluded	Rationale/ justification
Medical Therapy	None	
ICD	NYHA IV	Minimal IPD data available from clinical trials (of 12,638 patients included in IPD database only 77 (0.6%) were NYHA IV and randomised to an ICD)
CRT-P	NYHA I/II	Minimal IPD data available from clinical trials (of 12,638 patients included in IPD database only 74 (0.6%) were NYHA I-II and randomised to a CRT-P)
	QRS duration<120ms	Prolonged QRS duration required for consideration of device insertion. No evidence of benefit from CRT in patients with normal QRS duration
CRT-D	QRS duration<120ms	Prolonged QRS duration required for consideration of device insertion. No evidence of benefit from CRT in patients with normal QRS duration

## Appendix 2: List of studies contributing information to all-cause hospitalisation and health related quality of life analyses

### All-cause hospitalisation

Abraham WT, Fisher WG, Smith AL, DeLurgio DB, Leon AR, Loh E et al. Cardiac resynchronization in chronic heart failure. *New England Journal of Medicine* 2002; 346(24):1845-1853.

Bardy GH, Lee KL, Mark DB, Poole JE, Packer DL, Boineau R et al. Amiodarone or an implantable cardioverter-defibrillator for congestive heart failure.[Erratum appears in N Engl J Med. 2005 May 19;352(20):2146]. *New England Journal of Medicine* 2005; 352(3):225-237.

Beshai JF, Grimm RA, Nagueh SF, Baker JH, Beau SL, Greenberg SM et al. Cardiac-resynchronization therapy in heart failure with narrow QRS complexes. *New England Journal of Medicine* 2007; 357(24):2461-2471.

Bristow MR, Saxon LA, Boehmer J, Krueger S, Kass DA, De MT et al. Cardiac-resynchronization therapy with or without an implantable defibrillator in advanced chronic heart failure. *New England Journal of Medicine* 2004; 350(21):2140-2150.

Cleland JG, Daubert JC, Erdmann E, Freemantle N, Gras D, Kappenberger L et al. The effect of cardiac resynchronization on morbidity and mortality in heart failure. *New England Journal of Medicine* 2005; 352(15):1539-1549.

Higgins SL, Hummel JD, Niazi IK, Giudici MC, Worley SJ, Saxon LA et al. Cardiac Resynchronization Therapy for the Treatment of Heart Failure in Patients with Intraventricular Conduction Delay and Malignant Ventricular Tachyarrhythmias. *Journal of the American College of Cardiology* 2003; 42(8):1454-1459.

Linde C, Abraham WT, Gold MR, St John SM, Ghio S, Daubert C et al. Randomized trial of cardiac resynchronization in mildly symptomatic heart failure patients and in asymptomatic patients with left ventricular dysfunction and previous heart failure symptoms. *Journal of the American College of Cardiology* 2008; 52(23):1834-1843.

Moss A. MADIT-CRT: The multicentre automatic defibrillator implantation trial-cardiac resynchronization therapy. *European Journal of Heart Failure* 2009; 11(12):1217-1219.

RHYTHM ICD. St. Jude Medical® Epic™ HF System including the Epic™ HF Model V-338 Cardiac Resynchronization Therapy Defibrillator, the Aescula™ LV Model 1055K Lead, the QuickSite™ LV Model 1056K Lead, and the Model 3307 v4.5m Programmer Software - P030054. US Food and Drug Administration



1  
2  
3 Tang AS, Wells GA, Talajic M, Arnold MO, Sheldon R, Connolly S et al. Cardiac-  
4 resynchronization therapy for mild-to-moderate heart failure. *New England Journal of*  
5 *Medicine* 2010; 363(25):2385-2395.  
6  
7

8  
9 Young JB, Abraham WT, Smith AL, Leon AR, Lieberman R, Wilkoff B et al. Combined  
10 cardiac resynchronization and implantable cardioversion defibrillation in advanced chronic  
11 heart failure: the MIRACLE ICD Trial. *JAMA : the journal of the American Medical*  
12 *Association* 2003; 289:2685-2694.  
13  
14

### 15 16 **Health Related Quality of Life**

17 Cleland JG, Daubert JC, Erdmann E, Freemantle N, Gras D, Kappenberger L et al. The  
18 effect of cardiac resynchronization on morbidity and mortality in heart failure. *New England*  
19 *Journal of Medicine* 2005; 352(15):1539-1549.  
20  
21

22  
23 Moss A. MADIT-CRT: The multicentre automatic defibrillator implantation trial-cardiac  
24 resynchronization therapy. *European Journal of Heart Failure* 2009; 11(12):1217-1219.  
25  
26

27 Tang AS, Wells GA, Talajic M, Arnold MO, Sheldon R, Connolly S et al. Cardiac-  
28 resynchronization therapy for mild-to-moderate heart failure. *New England Journal of*  
29 *Medicine* 2010; 363(25):2385-2395.  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60

### Appendix 3: Additional model parameters

Table S2: Background medication by NYHA class (% patients receiving each drug)

	NYHA I	NYHA II	NYHA III	NYHA IV
Atorvastatin	20%	20%	20%	20%
Simvastatin	55%	55%	55%	55%
Warfarin	10%	15%	25%	40%
Clopidogrel	15%	15%	15%	15%
Ramipril	90%	90%	90%	90%
Carvedilol	85%	85%	75%	70%
Spironolactone	0%	30%	30%	30%
Digoxin	5%	25%	25%	25%
Furosemide	75%	80%	90%	95%
Eplerenone	0%	30%	30%	30%

Table S3: Medication purchase costs (all data taken from the British National Formulary<sup>24</sup>, cost year 2012)

Drug	Tablets per pack	Daily dose	Pack price
Atrovastatin (Liptor®)	28	10mg	£13.00
Simvastatin	28	10mg	£0.90
	28	20mg	£1.01
	28	40mg	£1.32
	28	80mg	£2.29
Warfarin	28	0.5mg	£1.49
	28	1mg	£0.93
Clopidigrel	30	75mg	£3.40
	28	75mg	£3.17
Ramipril	28	1.25mg	£1.10
	28	2.5mg	£1.18
	28	5mg	£1.25
	28	10mg	£1.41
Carvedilol	28	3.125mg	£1.10
	28	6.25mg	£1.25
	28	12.5mg	£1.37
	28	25mg	£1.84
Spironolactone	28	25mg	£1.55
	28	50mg	£2.11
	28	100mg	£2.46
Digoxin	28	62.5	£2.03
	28	125	£1.12
	28	250	£1.13
Furosemide	28	20	£0.81
	28	40	£0.84
	28	500	£4.05
Eplerenone	28	25	£42.72

Table S4: Hospitalisation event costs (cost year 2012)

Item	Cost	Source
Day in hospital (HF)	£655.71	NHS Schedule of reference costs <sup>16,22</sup>
Day in hospital (non-HF)	£699.50	NHS Schedule of reference costs <sup>16,22</sup>
Day in hospital (leads)	£794.41	NHS Schedule of reference costs <sup>16,22</sup>
HF hospitalisation event	£2,295	NHS Schedule of reference costs <sup>16,22</sup>
Non-HF hospitalisation event	£2,448	NHS Schedule of reference costs <sup>16,22</sup>
Outpatient visits <sup>a</sup>	£110.00	Unit costs of health and social care <sup>16,23</sup>

a) Applied every six months to all patients alive regardless of device option in addition to any other hospitalisation event costs.

Table S5: ICD and CRT system costs (source Association of British Healthcare Industries unless otherwise stated, cost year 2012)

Item	Cost	Source
<i>System costs</i>		
CRT-P whole system costs (device and leads)	£3,411	Association of British Healthcare Industries*
CRT-D whole system costs (device and leads)	£12,293	Association of British Healthcare Industries*
ICD whole system costs (device and leads)	£9,692	Association of British Healthcare Industries*
CRT Leads	£510	Association of British Healthcare Industries*
CRT-P pulse generator	£2,600	Association of British Healthcare Industries*
CRT-D pulse generator	£11,752	Association of British Healthcare Industries*
ICD generator	£9,149	Association of British Healthcare Industries*
<i>UK Tariff values</i>		
CRT-P	£8,281	NHS Schedule of reference costs <sup>16,22</sup>
ICD/CRT-D non-purchase costs	£5,556	NHS Schedule of reference costs <sup>16,22</sup>
Revisions not requiring new device	£2,748	NHS Schedule of reference costs <sup>16,22</sup>

\* Data on file

Table S6: Device costs used in the model (cost year 2012)

Item	Cost	Components
Initial implant operation (ICD)	£15,248	ABHI system costs (incl. leads) and UK tariff EA12Z
Initial implant operation (CRT-P)	£8,281	UK Tariff E07Z
Initial implant operation (CRT-D)	£17,849	ABHI system costs (incl. leads) and UK tariff EA12Z
Replacement (ICD)	£14,705	ABHI system costs (excl. leads) and UK tariff EA12Z
Replacement (CRT-P)	£8,281	UK Tariff E07Z
Replacement (CRT-D)	£17,308	ABHI System costs (excl. leads)* and UK tariff EA12Z
Device related infection (ICD)	£18,964	See footnote
Device related infection (CRT-P)	£12,541	See footnote
Device related infection (CRT-D)	£21,568	See footnote
Battery replacement (ICD)	£12,004	ABHI generator costs (excl. leads) and UK tariff EA39Z
Battery replacement (CRT-P)	£8,381	UK Tariff EA07Z
Battery replacement (CRT-D)	£14,672	ABHI generator costs (excl. leads) and UK tariff EA39Z

As per previous NICE appraisal of CRT, for the purpose of costing we have assumed that treatment of a device related infection involves explanation of the existing device and a *de novo* device reimplantation as well as an additional outpatient visit. Detailed breakdown of the relevant resource use protocol can be found in the ABHI NICE submission dossier.<sup>16</sup>

Table S7: Parameter estimates which to inform Weibull models (time to first device failure)<sup>a</sup>

Parameter	ICD	CRT-P	CRT-D
Log-Lambda	-15.784	-14.287	-15.465
Gamma	1.943	1.689	1.935

a) Full details on source data and the modelling of device longevity to be found in the relevant NICE submission<sup>25</sup>

## Appendix 4: Clinical baseline risk equations

Table S8: Preferred baseline risk models (all-cause mortality and hospitalisation)

Variable	All-cause mortality (Weibull model)			All-cause hospitalisation (negative binomial model)		
	Coefficient	Hazard ratio <sup>a</sup>	P-value	Coefficient	Hazard ratio <sup>b</sup>	P-value
Age (per year), time-dependent covariate	0.03	1.02	<0.001	0.02	1.00	0.004
Male gender	0.24	1.24	0.003	N/A	N/A	N/A
NYHA III	0.62	1.74	<0.001	0.74	2.10	<0.001
NYHA IV	1.30	3.20	<0.001	1.48	4.41	<0.001
Ischaemic aetiology	0.37	1.39	<0.001	0.09	1.09	0.031
QRS duration <120ms	-0.20	0.84	0.002	N/A	N/A	N/A
QRS duration ≥120ms and <150ms	N/A	N/A	N/A	0.20	1.22	<0.001
QRS duration ≥150ms	N/A	N/A	N/A	0.06	1.06	<0.001
LVEF>20% and ≤25%	-0.26	0.79	0.001	N/A	N/A	N/A
LVEF>25% and ≤30%	-0.34	0.74	<0.001	N/A	N/A	N/A
LVEF>30%	-0.65	0.56	<0.001	N/A	N/A	N/A
log(scale)	10.09	N/A	<0.001	N/A	N/A	N/A
log(shape)	0.12	N/A	<0.001	N/A	N/A	N/A
Constant	N/A	N/A	N/A	-2.73	N/A	N/A

a) Hazard ratio =  $\exp(\text{coefficient}/\text{shape})$ ; b) hazard ratio =  $\exp(\text{coefficient})$ . N/A = not applicable

Table S9: Negative Binomial Regression coefficients used to predict baseline utility

Covariable	Coefficient	Hazard ratio <sup>a</sup>	p-value
NYHA = III	0.4667	1.595	<0.001
NYHA = IV*	0.7721	2.164	0.117
Age	-0.0061	0.994	0.003
Ischaemic aetiology	0.1427	1.153	0.001
Gender= Male	-0.2296	0.794	<0.001
Constant	3.5271	N/A	N/A

a) Hazard ratio = $\exp(\text{coefficient})$ ;



## Appendix 5: Long term survival extrapolation and lifetime hospitalisation counts

Table S10: Predicted overall survival and lifetime hospitalisation event estimates (Medical Therapy, where included as a treatment option)

Pt. group	Predicted overall survival							Hospitalisation count (lifetime)
	0 yrs	2 yrs	4 yrs	6 yrs	8 yrs	10 yrs	Median	
<i>Individuals without LBBB morphology</i>								
NYHA I, QRS duration < 120ms <sup>a</sup>	100.0%	87.5%	74.5%	62.0%	51.3%	42.0%	8.96	1.58
NYHA I, QRS duration ≥ 120ms and < 150ms <sup>a</sup>	100.0%	82.0%	64.6%	49.3%	37.5%	28.0%	6.37	1.44
NYHA I, QRS duration ≥ 150ms <sup>a</sup>	100.0%	80.8%	62.7%	46.9%	35.0%	25.7%	6.06	1.19
NYHA II, QRS duration < 120ms	100.0%	89.3%	77.9%	66.8%	57.0%	48.3%	10.61	1.78
NYHA II, QRS duration ≥ 120ms and < 150ms	100.0%	83.4%	67.1%	52.5%	40.8%	31.4%	7.00	1.54
NYHA II, QRS duration ≥ 150ms	100.0%	82.4%	65.4%	50.4%	38.7%	29.4%	6.66	1.28
NYHA III, QRS duration < 120ms	100.0%	78.3%	59.0%	43.2%	31.9%	23.4%	5.78	2.14
NYHA III, QRS duration ≥ 120ms and < 150ms	100.0%	69.8%	46.3%	29.7%	19.3%	12.6%	4.08	1.91
NYHA III, QRS duration ≥ 150ms	100.0%	66.3%	41.5%	25.0%	15.4%	9.5%	3.58	1.49
NYHA IV, QRS duration < 120ms	100.0%	52.0%	25.3%	11.7%	5.5%	2.6%	2.32	1.94
NYHA IV, QRS duration ≥ 120ms and < 150ms	100.0%	45.5%	19.9%	8.7%	4.1%	2.0%	2.02	2.03
NYHA IV, QRS duration ≥ 150ms	100.0%	42.6%	17.0%	6.5%	2.6%	1.0%	1.82	1.59
<i>Individuals with LBBB morphology</i>								
NYHA I, QRS duration ≥ 120ms and < 150ms <sup>a</sup>	100.0%	83.4%	67.2%	52.7%	41.2%	31.9%	7.23	1.58
NYHA I, QRS duration ≥ 150ms <sup>a</sup>	100.0%	82.1%	64.8%	49.6%	37.8%	28.5%	6.56	1.27

NYHA II, QRS duration $\geq$ 120ms and <150ms	100.0%	84.8%	69.7%	55.9%	44.8%	35.5%	7.82	1.66
NYHA II, QRS duration $\geq$ 150ms	100.0%	85.0%	70.2%	56.5%	45.4%	36.2%	7.90	1.45
NYHA III, QRS duration $\geq$ 120ms and <150ms	100.0%	69.8%	46.6%	30.3%	20.1%	13.5%	4.19	1.94
NYHA III, QRS duration $\geq$ 150ms	100.0%	70.3%	47.2%	30.8%	20.4%	13.6%	4.20	1.68
NYHA IV, QRS duration $\geq$ 120ms and <150ms	100.0%	46.8%	21.1%	9.7%	5.0%	2.7%	2.16	2.10
NYHA IV, QRS duration $\geq$ 150ms	100.0%	45.6%	20.1%	8.8%	4.2%	2.0%	2.03	1.73

a) Results in NYHA I and IV patients are based on relatively low patient numbers and may be subject to bias due to the nature of trial inclusion criteria for NYHA I patients. For further detail see main text.

Table S11: Predicted overall survival and lifetime hospitalisation event estimates (ICD, where included as a treatment option)

Pt. group	Predicted overall survival							Hospitalisation count (lifetime)
	0 yrs	2 yrs	4 yrs	6 yrs	8 yrs	10 yrs	Median	
<i>Individuals without LBBB morphology</i>								
NYHA I, QRS duration < 120ms <sup>a</sup>	100.0%	90.5%	80.2%	69.9%	60.6%	51.8%	11.08	1.47
NYHA I, QRS duration ≥ 120ms and < 150ms <sup>a</sup>	100.0%	88.3%	76.1%	64.1%	53.8%	44.1%	9.25	1.52
NYHA I, QRS duration ≥ 150ms <sup>a</sup>	100.0%	86.1%	71.9%	58.5%	47.4%	37.5%	8.06	1.19
NYHA II, QRS duration < 120ms	100.0%	91.9%	83.0%	73.9%	65.6%	57.6%	12.83	1.63
NYHA II, QRS duration ≥ 120ms and < 150ms	100.0%	89.2%	77.7%	66.4%	56.5%	47.0%	9.90	1.59
NYHA II, QRS duration ≥ 150ms	100.0%	87.4%	74.3%	61.8%	51.2%	41.6%	8.86	1.27
NYHA III, QRS duration < 120ms	100.0%	83.1%	66.9%	52.7%	41.6%	32.4%	7.32	2.05
NYHA III, QRS duration ≥ 120ms and < 150ms	100.0%	79.4%	60.7%	45.2%	33.7%	24.5%	6.00	2.10
NYHA III, QRS duration ≥ 150ms	100.0%	74.8%	53.4%	37.0%	25.8%	17.6%	4.89	1.55
<i>Individuals with LBBB morphology</i>								
NYHA I, QRS duration ≥ 120ms and < 150ms <sup>a</sup>	100.0%	88.2%	75.8%	63.8%	53.5%	44.1%	9.48	1.55
NYHA I, QRS duration ≥ 150ms <sup>a</sup>	100.0%	86.0%	71.7%	58.3%	47.2%	37.5%	8.12	1.20
NYHA II, QRS duration ≥ 120ms and < 150ms	100.0%	89.0%	77.4%	66.0%	56.1%	46.9%	10.05	1.60
NYHA II, QRS duration ≥ 150ms	100.0%	88.2%	75.9%	64.0%	53.9%	44.7%	9.60	1.33
NYHA III, QRS duration ≥ 120ms and < 150ms	100.0%	77.3%	57.5%	41.7%	30.5%	22.0%	5.61	1.98
NYHA III, QRS duration ≥ 150ms	100.0%	75.3%	54.4%	38.3%	27.2%	19.1%	5.11	1.58

a) Results in NYHA I and IV patients are based on relatively low patient numbers and may be subject to bias due to the nature of trial inclusion criteria for NYHA I patients. For further detail see main text.

Table S12: Predicted overall survival and lifetime hospitalisation event estimates (CRT-P, where included as a treatment option)

Pt. group	Predicted overall survival							Hospitalisation count (lifetime)
	0 yrs	2 yrs	4 yrs	6 yrs	8 yrs	10 yrs	Median	
<i>Individuals without LBBB morphology</i>								
NYHA III, QRS duration $\geq 120$ ms and $< 150$ ms	100.0%	71.4%	48.4%	31.7%	21.0%	13.9%	4.29	1.35
NYHA III, QRS duration $\geq 150$ ms	100.0%	71.9%	49.0%	32.1%	21.2%	13.8%	4.31	1.19
NYHA IV, QRS duration $\geq 120$ ms and $< 150$ ms	100.0%	48.5%	22.7%	10.7%	5.4%	2.8%	2.21	1.33
NYHA IV, QRS duration $\geq 150$ ms	100.0%	50.9%	24.2%	11.1%	5.3%	2.4%	2.27	1.18
<i>Individuals with LBBB morphology</i>								
NYHA III, QRS duration $\geq 120$ ms and $< 150$ ms	100.0%	74.9%	53.8%	37.7%	26.7%	18.7%	5.05	1.54
NYHA III, QRS duration $\geq 150$ ms	100.0%	78.7%	59.6%	44.0%	32.6%	23.6%	5.82	1.50
NYHA IV, QRS duration $\geq 120$ ms and $< 150$ ms	100.0%	54.8%	28.6%	14.8%	8.1%	4.6%	2.67	1.54
NYHA IV, QRS duration $\geq 150$ ms	100.0%	58.7%	32.8%	17.9%	10.1%	5.6%	2.90	1.45

Table S13: Predicted overall survival and lifetime hospitalisation event estimates (CRT-D, where included as a treatment option)

Pt. group	Predicted overall survival							Hospitalisation count (lifetime)
	0 yrs	2 yrs	4 yrs	6 yrs	8 yrs	10 yrs	Median	
<i>Individuals without LBBB morphology</i>								
NYHA I, QRS duration $\geq$ 120ms and <150ms <sup>a</sup>	100.0%	87.0%	73.5%	60.6%	49.6%	39.7%	8.37	1.24
NYHA I, QRS duration $\geq$ 150ms <sup>a</sup>	100.0%	87.7%	74.8%	62.2%	51.5%	41.5%	8.71	1.10
NYHA II, QRS duration $\geq$ 120ms and <150ms	100.0%	88.1%	75.6%	63.4%	52.9%	43.3%	9.15	1.31
NYHA II, QRS duration $\geq$ 150ms	100.0%	88.7%	76.8%	65.1%	54.8%	45.1%	9.48	1.16
NYHA III, QRS duration $\geq$ 120ms and <150ms	100.0%	77.8%	58.0%	42.0%	30.5%	21.6%	5.52	1.72
NYHA III, QRS duration $\geq$ 150ms	100.0%	77.5%	57.5%	41.2%	29.6%	20.6%	5.36	1.46
NYHA IV, QRS duration $\geq$ 120ms and <150ms	100.0%	57.7%	31.7%	17.3%	9.8%	5.5%	2.86	1.95
NYHA IV, QRS duration $\geq$ 150ms	100.0%	58.9%	32.5%	17.2%	9.3%	4.7%	2.81	1.68
<i>Individuals with LBBB morphology</i>								
NYHA I, QRS duration $\geq$ 120ms and <150ms <sup>a</sup>	100.0%	89.5%	78.2%	67.1%	57.3%	47.9%	10.18	1.42
NYHA I, QRS duration $\geq$ 150ms <sup>a</sup>	100.0%	89.9%	79.0%	68.0%	58.3%	48.6%	10.18	1.23
NYHA II, QRS duration $\geq$ 120ms and <150ms	100.0%	90.5%	80.2%	69.9%	60.7%	51.6%	10.99	1.49
NYHA II, QRS duration $\geq$ 150ms	100.0%	91.6%	82.5%	73.1%	64.6%	55.8%	11.85	1.35
NYHA III, QRS duration $\geq$ 120ms and <150ms	100.0%	80.3%	62.2%	47.0%	35.7%	26.4%	6.32	1.90
NYHA III, QRS duration $\geq$ 150ms	100.0%	82.8%	66.4%	51.9%	40.6%	30.8%	7.02	1.77
NYHA IV, QRS duration $\geq$ 120ms and <150ms	100.0%	62.9%	37.6%	22.0%	13.3%	8.0%	3.37	2.21
NYHA IV, QRS duration $\geq$ 150ms	100.0%	65.4%	40.8%	24.8%	15.4%	9.1%	3.56	2.02

1  
2  
3 a) Results in NYHA I and IV patients are based on relatively low patient numbers and may be subject to bias due to the nature of trial inclusion criteria for NYHA I patients. For  
4 further detail see main text.  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47

Confidential: For Review Only

## Appendix 6: Results from additional economic sensitivity analyses

Table S14: Cost-effectiveness results generated using constant treatment effects


Pt. group	C-E Sequence				ICERs			
	1st	2nd	3 <sup>rd</sup>	4th	1 <sup>st</sup>	2nd	3 <sup>rd</sup>	4 <sup>th</sup>
<i>Individuals without LBBB morphology</i>								
NYHA I, QRS duration < 120ms <sup>a</sup>	MT	ICD	N/A	N/A	Referent	£17,799	N/A	N/A
NYHA I, QRS duration ≥ 120ms and < 150ms <sup>a</sup>	MT	CRTD	ICD	N/A	Referent	Dominated	£12,991	N/A
NYHA I, QRS duration ≥ 150ms <sup>a</sup>	MT	ICD	CRTD	N/A	Referent	£17,390	£19,372	N/A
NYHA II, QRS duration < 120ms	MT	ICD	N/A	N/A	Referent	£17,305	N/A	N/A
NYHA II, QRS duration ≥ 120ms and < 150ms	MT	CRTD	ICD	N/A	Referent	Dominated	£13,210	N/A
NYHA II, QRS duration ≥ 150ms	MT	ICD	CRTD	N/A	Referent	£16,577	£20,796	N/A
NYHA III, QRS duration < 120ms	MT	ICD	N/A	N/A	Referent	£24,187	N/A	N/A
NYHA III, QRS duration ≥ 120ms and < 150ms	MT	CRTD	ICD	CRTD	Referent	£17,350	Ext Dominated	£20,117
NYHA III, QRS duration ≥ 150ms	MT	ICD	CRTD	CRTD	Referent	Dominated	£12,008	£20,692
NYHA IV, QRS duration < 120ms	MT	N/A	N/A	N/A	Referent	N/A	N/A	N/A
NYHA IV, QRS duration ≥ 120ms and < 150ms	MT	CRTD	CRTD	N/A	Referent	£21,805	£37,981	N/A
NYHA IV, QRS duration ≥ 150ms	MT	CRTD	CRTD	N/A	Referent	£16,271	£33,035	N/A
<i>Individuals with LBBB morphology</i>								
NYHA I, QRS duration ≥ 120ms and < 150ms <sup>a</sup>	MT	ICD	CRTD	N/A	Referent	£16,438	£18,239	N/A
NYHA I, QRS duration ≥ 150ms <sup>a</sup>	MT	ICD	CRTD	N/A	Referent	Ext Dominated	£14,058	N/A
NYHA II, QRS duration ≥ 120ms and < 150ms	MT	ICD	CRTD	N/A	Referent	Ext Dominated	£16,318	N/A

NYHA II, QRS duration $\geq$ 150ms	MT	ICD	CRTD	N/A	Referent	Ext Dominated	£13,510	N/A
NYHA III, QRS duration $\geq$ 120ms and $<$ 150ms	MT	ICD	CRTD	CRTD	Referent	Dominated	£12,071	£20,255
NYHA III, QRS duration $\geq$ 150ms	MT	ICD	CRTD	CRTD	Referent	Dominated	£8,935	£22,075
NYHA IV, QRS duration $\geq$ 120ms and $<$ 150ms	MT	CRTD	CRTD	N/A	Referent	£17,519	£33,833	N/A
NYHA IV, QRS duration $\geq$ 150ms	MT	CRTD	CRTD	N/A	Referent	£13,733	£36,328	N/A

a) Results in NYHA I and IV patients are based on relatively low patient numbers and may be subject to bias due to the nature of trial inclusion criteria for NYHA I patients. For further detail see main text.



Figure S1: Graphic display of cost-effective option across cost-effectiveness threshold values in patients with LBBB morphology (sensitivity analyses – constant all-cause mortality and HRQoL treatment effects)

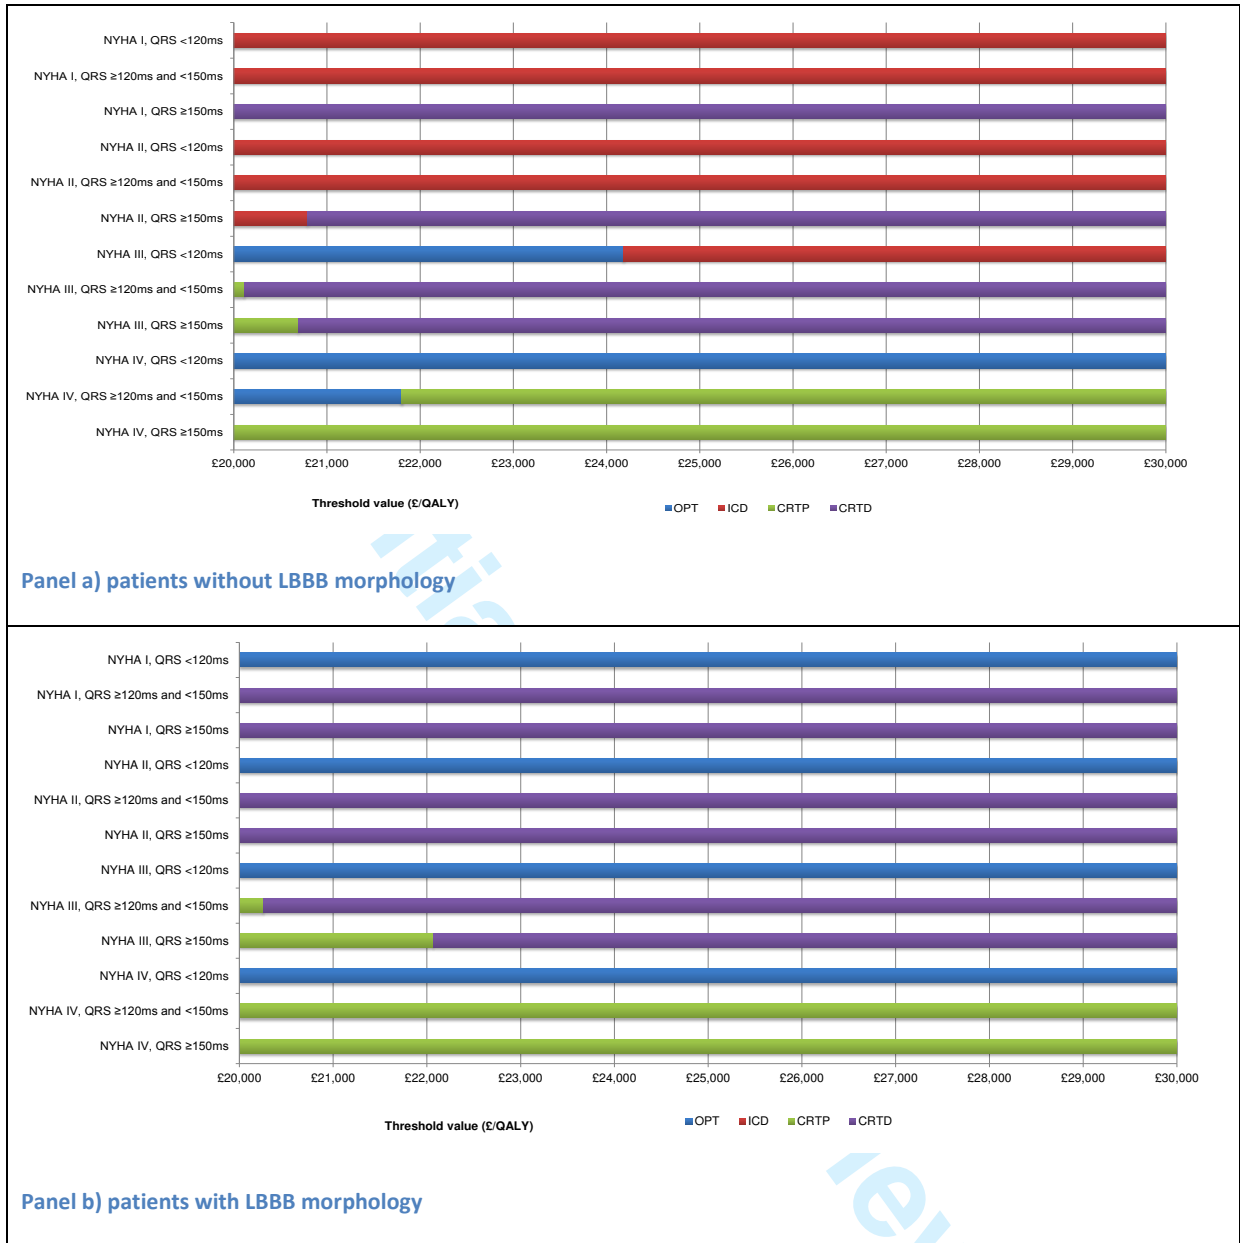

Legend: Results in NYHA I patients are based on relatively low patient numbers and may be subject to bias due to the nature of trial inclusion criteria for NYHA I patients. For further detail see main text.