



UNIVERSITY OF LEEDS

This is a repository copy of *Jacobian-Based Iterative Method for Magnetic Localization in Robotic Capsule Endoscopy*.

White Rose Research Online URL for this paper:
<http://eprints.whiterose.ac.uk/103408/>

Version: Accepted Version

Article:

Di Natali, C, Beccani, M, Simaan, N et al. (1 more author) (2016) Jacobian-Based Iterative Method for Magnetic Localization in Robotic Capsule Endoscopy. *IEEE Transactions on Robotics*, 32 (2). pp. 327-338. ISSN 1552-3098

<https://doi.org/10.1109/TRO.2016.2522433>

(c) 2016 IEEE. Personal use of this material is permitted. Permission from IEEE must be obtained for all other users, including reprinting/ republishing this material for advertising or promotional purposes, creating new collective works for resale or redistribution to servers or lists, or reuse of any copyrighted components of this work in other works.

Reuse

Unless indicated otherwise, fulltext items are protected by copyright with all rights reserved. The copyright exception in section 29 of the Copyright, Designs and Patents Act 1988 allows the making of a single copy solely for the purpose of non-commercial research or private study within the limits of fair dealing. The publisher or other rights-holder may allow further reproduction and re-use of this version - refer to the White Rose Research Online record for this item. Where records identify the publisher as the copyright holder, users can verify any specific terms of use on the publisher's website.

Takedown

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing eprints@whiterose.ac.uk including the URL of the record and the reason for the withdrawal request.



eprints@whiterose.ac.uk
<https://eprints.whiterose.ac.uk/>

Jacobian-based Iterative Method For Magnetic Localization in Robotic Capsule Endoscopy

Christian Di Natali*, *Student Member, IEEE*, Marco Beccani, *Student Member, IEEE*,
Nabil Simaan, *Senior Member, IEEE* and Pietro Valdastri, *Senior Member, IEEE*

Abstract—The purpose of this study is to validate a Jacobian-based iterative method for real-time localization of magnetically controlled endoscopic capsules. The proposed approach applies finite element solutions to the magnetic field problem and least squares interpolations to obtain closed-form and fast estimates of the magnetic field. By defining a closed-form expression for the Jacobian of the magnetic field relative to changes in the capsule pose, we are able to obtain an iterative localization at a faster computational time when compared with prior works, without suffering from the inaccuracies stemming from dipole assumptions. This new algorithm can be used in conjunction with an absolute localization technique that provides initialization values at a slower refresh rate.

The proposed approach was assessed via simulation and experimental trials, adopting a wireless capsule equipped with a permanent magnet, six magnetic field sensors, and an inertial measurement unit. The overall refresh rate, including sensor data acquisition and wireless communication, was 7 ms, thus enabling closed-loop control strategies for magnetic manipulation running faster than 100 Hz. The average localization error, expressed in cylindrical coordinates, was below 7 mm in both the radial and axial components, and 5° in the azimuthal component. The average error for the capsule orientation angles, obtained by fusing gyroscope and inclinometer measurements, was below 5° .

I. INTRODUCTION

Wireless capsule endoscopy (WCE) allows physicians to visualize internal organs for diagnosis and potentially for intervention. This paper focuses on creating a modeling and algorithmic framework for localization of magnetically actuated WCEs. All the existing platforms for remote magnetic manipulation of a WCE inside the patient's body operate in open loop [1], i.e. the capsule pose (i.e., position and orientation) is not tracked and used for control feedback purposes. Position control of WCEs is typically based on the assumption that the permanent magnet inside the capsule aligns with the external magnetic field. Pose tracking of the WCE would allow the capsule to automatically optimize magnetic coupling to

maintain effective magnetic actuation, enabling the user to detect if the capsule is not following the expected trajectory (i.e., the capsule is trapped within a tissue fold), and to take appropriate countermeasures for re-establishing an effective motion. An example of position closed-loop control for a magnetically manipulated WCE is presented in [2], where optical tracking with external cameras is adopted to localize the capsule. To apply these results in a clinical setting and move toward the closed-loop manipulation of magnetic WCE position and orientation, online pose tracking without line-of-sight is crucial [3, 4].

Known methods for WCE pose tracking were designed largely for diagnostic purposes (i.e., to associate a lesion visualized by the capsule to its position inside the patient's body) [5, 6, 7, 8], and are not compatible with magnetic manipulation due to electromagnetic interference with the external source of the driving field. Recently, a number of groups working on robotic magnetic manipulation of WCE began studying localization strategies that are compatible with magnetic manipulation. These works implement localization based on measuring the magnetic field at the WCE via magnetic field sensors. Generally, these works rely on absolute localization using simple dipole models (e.g. [9, 10]) or lookup tables based on finite element solutions to the exact magnetic field (e.g. [11, 3]). The simple dipole models provide limited localization performance when the WCE is close to the magnetic field source. They work best when the WCE workspace is far away from the driving magnet. However, to maximize the magnetic coupling, the WCE should ideally operate as close as possible to the driving magnet. The drawbacks of lookup table based localization are the slow refresh rate and large memory requirements.

The performance of current WCE localization algorithms provide modest localization accuracy within limited workspace. In [10], multiple measurements taken of the capsule moving along its main axis toward the external magnet allows the user to obtain the position in three degrees of freedom (DOF) with an error below 4 mm when the capsule is within 6 cm of an external magnet. Continuous rotation of the capsule by an external revolving magnetic field combined with on-board magnetic field sensing [9] allows detection of the capsule position and orientation with an average error of 11 mm and 11 degrees within the operative workspace. Real-time systems, such as [11, 3, 4], leverage sensor fusion (i.e., inertial and magnetic field sensing) and search within pre-compiled finite element magnetic maps. In particular, the method proposed in [11] achieves a refresh rate of 50 ms

Research reported in this publication was supported in part by the National Institute of Biomedical Imaging And Bioengineering of the National Institutes of Health under Award Number R01EB018992, and in part by the National Science Foundation under grants CNS-1239355 and IIS-1453129. Any opinions, findings and conclusions or recommendations expressed in this material are those of the authors and do not necessarily reflect the views of the NIH or the NSF. *Asterisk indicates corresponding author.*

C. Di Natali, M. Beccani, and P. Valdastri are with the STORM Lab, Department of Mechanical Engineering, Vanderbilt University, Nashville, TN 37235, USA (e-mail: christian.di.natali@vanderbilt.edu; marco.beccani@vanderbilt.edu; p.valdastri@vanderbilt.edu).

N. Simaan is with the ARMA Lab, Department of Mechanical Engineering, Vanderbilt University, Nashville, TN 37235, USA (e-mail: n.simaan@vanderbilt.edu).

and a position error of 10 mm within a 12 cm workspace. Better performances are obtained in [4], where refresh rate goes down to 30 ms and the error drops below 6 mm within a 15 cm workspace. Finally, in our previous work [4], the sensor data acquisition and the localization algorithm required 6.5 ms and 16 ms per loop, respectively. One of the aims of our proposed new localization method is to decrease computational time, thus achieving both sensor acquisition and localization within 10 ms, allowing the implementation of a 100 Hz WCE manipulation closed-loop control.

In this paper, we validate our proposed algorithm on a WCE localization setup that includes an extracorporeal magnetic field source that manipulates an intracorporeal WCE. The localization strategy proposed herein aims to provide the change in pose of a WCE with respect to an external magnetic field source having known position and orientation. Using a similar approach to that used in [11, 3, 4], the capsule is henceforth assumed to be equipped with an inertial measurement unit (IMU) and six orthogonal magnetic field sensors. When inertial data from IMU are integrated, as we propose in our method, drift becomes an issue over time. For this reason, our approach is best used in synergy with an absolute localization technique [3, 4] working at a slower refresh rate. In such a scheme, the absolute localization can repeatedly provide initialization values to our algorithm, thus preventing the integration error from exceeding a desired value.

The contribution of this paper stems from putting forward a new approach for WCE localization by using an iterative Jacobian-based method. To the best of our knowledge, iterative methods for WCE pose tracking that are compatible with magnetic manipulation have not been presented in prior works, partly because a complete analytical solution for the magnetic field is not available. To overcome this challenge, we apply finite element solutions to the magnetic field problem and least squares interpolations to obtain closed-form and fast estimates of the magnetic field. By defining a closed-form expression for the Jacobian of the magnetic field relative to changes in the WCE pose, we are able to obtain an iterative WCE localization method without suffering from the inaccuracies stemming from dipole assumptions and without the downside of a slow refresh rate.

II. METHOD

A. Iterative Method for Magnetic Localization

Our localization approach is inspired by Jacobian-based methods (also known as resolved rates methods stemming from [12]). These methods are commonly used in robotics to solve systems of nonlinear equations subject to the limitations of first-order linearization. In this paper, we assume that the refresh rate for pose tracking is fast enough that only small movements of the WCE may occur between subsequent pose measurements. We also assume that the orientation of the capsule is known through the algorithm described in Section III running on IMU data.

In order to apply an iterative method to magnetic localization, we need to consider the magnetic field, generated by

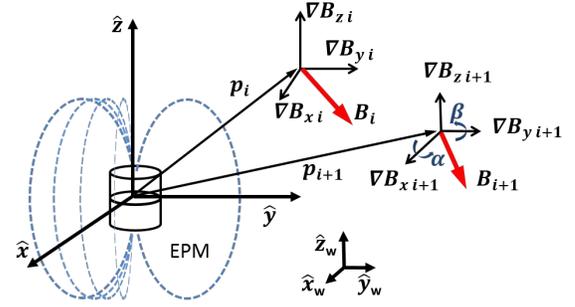


Fig. 1. Schematic representation of the source of magnetic field (External Permanent Magnet (EPM) in figure) and two sequential positions (i.e., \mathbf{p}_i and \mathbf{p}_{i+1}) of the capsule to be localized. The capsule orientational angles yaw and pitch are referred to as α and β , respectively.

a known source, as the following time-invariant non-linear mathematical expression:

$$\mathbf{B}_i = f(\mathbf{p}_i) \quad f(\mathbf{p}_i) : \mathbb{R}^3 \rightarrow \mathbb{R}^3. \quad (1)$$

This equation will be denoted as Magnetic Direct Relationship (MDR). Referring to Fig. 1, the MDR associates the coordinates of a point outside the magnetic field source $\mathbf{p}_i = [x_i, y_i, z_i]^T$ to a corresponding vector function of magnetic field values $\mathbf{B}_i = [B_{ix}, B_{iy}, B_{iz}]^T$.

If the capsule position changes from \mathbf{p}_i to \mathbf{p}_{i+1} during a time increment Δt , the displacement $\Delta \mathbf{p}$ produces a change in the magnetic field measurements from \mathbf{B}_i to \mathbf{B}_{i+1} according to (1). The partial derivative of the magnetic field vector, $\frac{\partial \mathbf{B}_i}{\partial \mathbf{p}}$, is given by:

$$\frac{\partial \mathbf{B}_i}{\partial \mathbf{p}} = \nabla_{\mathbf{p}} f(\mathbf{p}_i) = \begin{bmatrix} \frac{\partial B_x}{\partial p_x} & \frac{\partial B_x}{\partial p_y} & \frac{\partial B_x}{\partial p_z} \\ \frac{\partial B_y}{\partial p_x} & \frac{\partial B_y}{\partial p_y} & \frac{\partial B_y}{\partial p_z} \\ \frac{\partial B_z}{\partial p_x} & \frac{\partial B_z}{\partial p_y} & \frac{\partial B_z}{\partial p_z} \end{bmatrix}. \quad (2)$$

where $\nabla_{\mathbf{p}} f(\mathbf{p}_i)$ designates the gradient of f with respect to \mathbf{p} . Using (2) in a first-order Taylor series approximation, we obtain:

$$\mathbf{B}_{i+1} = \mathbf{B}_i + \frac{\partial \mathbf{B}_i}{\partial \mathbf{p}} \Delta \mathbf{p} = \mathbf{B}_i + \nabla_{\mathbf{p}} f(\mathbf{p}_i) \Delta \mathbf{p}. \quad (3)$$

The Magnetic Inverse Relationship (MIR), providing the current capsule position \mathbf{p}_{i+1} , can be derived by inverting (3):

$$\mathbf{p}_{i+1} = \mathbf{p}_i + \nabla_{\mathbf{p}} f^{-1}(\mathbf{p}_i) \Delta \mathbf{B}_i. \quad (4)$$

Moving from differential to the finite difference iterative method, $\frac{\partial \mathbf{B}}{\partial \mathbf{p}} \Delta \mathbf{p}$ is replaced by $\Delta \mathbf{B}_i$, where $\Delta \mathbf{B}_i$ is defined as $\Delta \mathbf{B}_i = (\mathbf{B}_{i+1} - \mathbf{B}_i)$. Also, according to [13], the gradient of a generic vectorial function, which is defined as $f(\mathbf{x}) : \mathbb{R}^n \rightarrow \mathbb{R}$, is the transpose of the Jacobian as: $\nabla_{\mathbf{x}} f(\mathbf{x}) = (\mathbf{J}_{\mathbf{x}} f(\mathbf{x}))^t$. Then, (4) becomes:

$$\mathbf{p}_{i+1} = \mathbf{p}_i + \mathbf{J}_p^{-1} \Delta \mathbf{B}_i, \quad (5)$$

where \mathbf{J}_p^{-1} is the inverse of the Jacobian.

An explicit formulation of the MDR (1) can be obtained by finite element integration of magnetic field models, as suggested in [14], while a numerical estimate can be provided by a standard finite element method (FEM) software package,

such as Comsol Multiphysics or ANSYS Maxwell. In the next subsections, we introduce a non-linear interpolation method for a data-set of magnetic field values related to the position \mathbf{p}_i . Then, the interpolation is used to provide an analytical expression of the MDR through modal representation, numerical algebra theory, and the Kronecker product. Finally, a first order resolved rates method using the Jacobian expression for the MIR is derived.

Figure 2 represents the proposed magnetic localization algorithm exploiting sensor fusion of magnetic field and inertial measurements. The magnetic field interpolation (also called magnetic field calibration) is achieved off-line, which leads to obtain the characteristic matrices \mathbf{A}_r and \mathbf{A}_z . Once the interpolation is obtained, the on-line algorithm takes as input the magnetic field, the inertial measurements, and the External Permanent Magnet (EPM) orientation, returning the capsule pose. The capsule position is referred to the EPM frame, whereas the orientation expressed in Euler angles is relative to the world frame. The blocks DMR-IMR –which stand for Direct and Inverse Magnetic Relationship– and the Iterative Jacobian Method are presented in Section II-B, while the three dimensional reconstruction is presented in Section II-C.

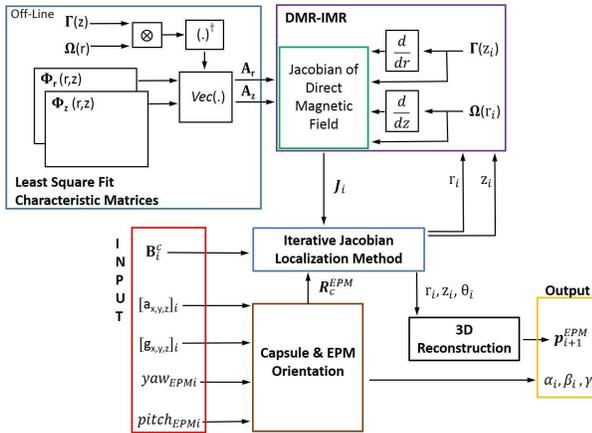


Fig. 2. Block diagram of the proposed iterative algorithm for WCE pose detection. In the diagram are displayed system input, output, Jacobian of the MDR, 3D reconstruction, and the off-line least square fit calibration, which leads to the characteristic matrices \mathbf{A}_r and \mathbf{A}_z .

B. Direct and Inverse Magnetic Relationship

The magnetic field of a cylindrical axially-magnetized permanent magnet exhibits cylindrical symmetry around its main axis (\hat{z}) [15, 16]. If such a magnet is used as the external source of a magnetic field for capsule manipulation, as suggested in our previous work [3, 4], the localization can take advantage of the symmetry to reduce the computational burden. In particular, the three-dimensional position tracking problem can be reduced to two dimensions (2D). Then, once the position in 2D is obtained, the third coordinate can be derived by sensor fusion as explained in Section II-C.

As represented in Fig. 3, the magnetic field is distributed around the main axis of symmetry of the EPM, \hat{z} , while B_θ – angular component of the magnetic field along θ – is null. The vector $\tilde{\mathbf{p}}_c = [r, \theta, z]^t$ represents a generic point on the

loci of points, whose location satisfies the condition of having the same magnetic field \mathbf{B}_c . This set of points of the locus generates a circumference Υ (represented in Fig. 3) that can be analytically described as $\Upsilon = [r, \theta, z] | r, z = const \in \mathbb{R}$, and $\theta \in 0 \rightarrow 2\pi$. We refer to $\tilde{\mathbf{p}}_c = [r, \theta, z]^t$ as the generic point on the loci, which is expressed in the three cylindrical coordinates, whereas \mathbf{p}_c lies on the plane \mathcal{H} and is obtained by applying a rotation about \hat{z} to $\tilde{\mathbf{p}}_c$. The plane \mathcal{H} is defined as: $\mathcal{H} = \mathbb{R}^2 : \{(r, z) | r, z \in \mathbb{R} \text{ and } \theta = 0\}$.

Considering the magnetic field applied on a generic point $\tilde{\mathbf{p}}_c$, its components are expressed as $\mathbf{B}_c = [B_r(r, z), B_\theta(r, z), B_z(r, z)]$, where $B_\theta(r, z) = 0$. Therefore, (1) could be furthermore simplified by defining the mathematical representation Ψ for the magnetic field \mathbf{B}_c . The magnetic field \mathbf{B}_c is given by the two-dimensional transformation Ψ for any given point $\tilde{\mathbf{p}}_c$ around the magnetic field source, such as $\Psi : \tilde{\mathbf{p}}_c \rightarrow \mathbf{B}_c$. $B_r(r, z)$ and $B_z(r, z)$ are two scalar values representing the radial and the axial component of the magnetic field vector, which are functions of axial and radial spatial coordinates with respect to the center of the EPM.

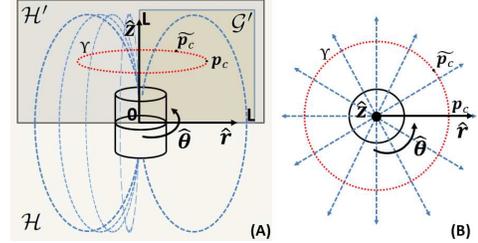


Fig. 3. Schematic view of the magnetic field distribution for a cylindrical axially-magnetized permanent magnet. (A) View of the \mathcal{H} planes, its subset \mathcal{H}' and the domain \mathcal{G}' , (B) shows the radial distribution of the magnetic field on the plane $[\hat{r}, \hat{\theta}]$.

The solution to the system of equations expressed by the transformation Ψ – in terms of both radial $B_r(r, z)$ and axial $B_z(r, z)$ magnetic field – is unique in the semi-domain \mathcal{H}' defined as in Fig. 3 (note that the semi-domain \mathcal{H}' can be either related to the south or the north pole of the cylindrical axially-magnetized EPM). Then, we define a finite domain \mathcal{G}' , where the magnetic field radial component B_r is always positive. On the other hand, if considering the domain \mathcal{H} , the transformation Ψ leads to two solutions in diagonally opposite quadrants in Fig. 3. Since the patient cannot be simultaneously above and below the magnet, we exclude one quadrant for practical implementation reasons. The region is a square plane having size L along \hat{r} and \hat{z} , where the spatial transformation $f(\mathbf{p}_c)$ in (1) is simplified and solvable as

$$\Psi(\mathbf{p}_c) : \mathbb{R}^2 \rightarrow \mathbb{R}^2$$

$$\text{where : } \mathbf{p}_c \in \mathcal{G}' : \mathcal{G}' = \{(r, z) \in [0, L]\} \quad (6)$$

The transformation $\Psi(\mathbf{p}_c)$ can be expressed by two scalar mathematical functions, each with two inputs. The two functions provide the magnetic field radial component as

$$B_r = \psi_r(r, z) : \mathbb{R}^2 \rightarrow \mathbb{R}, \quad (7)$$

and the magnetic field axial component as

$$B_z = \psi_z(r, z) : \mathbb{R}^2 \rightarrow \mathbb{R}. \quad (8)$$

The numerical solution of (7) and (8) can be obtained by either applying the Current Density Magnetic Model (CuDMM) or the Charge Density Magnetic Model (ChDMM), as demonstrated in [15, 16]. Then, the magnetic field values can be casted in two data matrices $\Phi_r \in \mathbb{R}^{m \times p}$ and $\Phi_z \in \mathbb{R}^{m \times p}$. These matrices represent the $m \times p$ magnetic field numerical solutions for any given position \mathbf{p}_c within \mathcal{G}' , where m is the number of magnetic field measurements taken along the $\hat{\mathbf{r}}$ direction and p is the number of magnetic field measurements taken along $\hat{\mathbf{z}}$. The collection of numerical solutions $[\Phi_r, \Phi_z]^T$ of (7) and (8), are expressed as in (9) and (10).

$$\Phi_r = [\Phi_{rij}(r_i, z_j)] \quad (9)$$

$$i \in \mathbb{N} : [1 \leq i \leq m]; j \in \mathbb{N} : [1 \leq j \leq p].$$

$$\Phi_z = [\Phi_{zij}(r_i, z_j)] \quad (10)$$

$$i \in \mathbb{N} : [1 \leq i \leq m]; j \in \mathbb{N} : [1 \leq j \leq p].$$

where Φ_{rij} and Φ_{zij} are the magnetic field values at position (i, j) , which could be generally expressed as Φ_{ij} . The single matrix element Φ_{ij} can be approximated by applying the modal representation defined in [17, 18, 19] as

$$\Phi_{ij} = \mathbf{B}_i(r, z) = \boldsymbol{\omega}(r)^T \mathbf{a}(z), \quad (11)$$

where : $(\mathbf{a}, \boldsymbol{\omega}) \in \mathbb{R}^n$.

The vector of the modal factors, $\mathbf{a}(z)$, can be expressed as

$$\mathbf{a}(z) = \mathbf{A}\boldsymbol{\gamma}(z), \quad (12)$$

where : $(\mathbf{A}, \boldsymbol{\gamma}) \in \mathbb{R}^n$.

In this equation, \mathbf{A} is the characteristic matrix of coefficients for the particular magnetic field shape, which together with the two orthogonal bases, $\boldsymbol{\omega} = \{\omega_0, \omega_1, \dots, \omega_n\}$ and $\boldsymbol{\gamma} = \{\gamma_0, \gamma_1, \dots, \gamma_q\}$, represents the interpolation functions that best numerically approximate the transformation Φ_{ij} over the domain of interest [20]. Once the interpolation functions $\boldsymbol{\omega}$ and $\boldsymbol{\gamma}$ are chosen (Section IV-A), and the characteristic matrices of coefficients \mathbf{A}_r and \mathbf{A}_z for radial and axial magnetic field respectively are derived, the interpolation problem can be easily solved. The best data-set interpolation is chosen by adopting the orthogonal function that minimizes the least square error between the reference measure $f(x)$ and the approximated value y^* , such as $\|f(x) - y^*\| < \delta$. Examples of orthogonal functions investigated in this study include standard polynomial functions, Chebyshev polynomials [19, 18], Fourier harmonic basis [20, 21] and composition of these.

In the following paragraph, we describe how to derive the characteristic matrices of coefficients \mathbf{A}_r and \mathbf{A}_z for the algebraic equations system in (11) and (12) by using the following matrix representation, as suggested in [19, 18]:

$$\Phi = \boldsymbol{\Omega}_{m \times n} \mathbf{A}_{n \times q} \boldsymbol{\Gamma}_{q \times p}, \quad (13)$$

where Φ is either the MDR solutions of Φ_r or Φ_z within $r, z \in [0 \rightarrow L]$, while $\boldsymbol{\Omega}$ and $\boldsymbol{\Gamma}$ are the modal basis matrices and constitute the collection of n orthogonal basis for $\boldsymbol{\Omega}$ and q orthogonal basis for $\boldsymbol{\Gamma}$. Finally, m and p are the number of values estimated in the domain $r \in [0, L]$ and $z \in [0, L]$, respectively.

The solutions for \mathbf{A}_r and \mathbf{A}_z can be obtained by applying the Kronecker product theory as in [19, 18, 22], where the symbol \otimes represents the Kronecker product of two matrices:

$$\text{Vec}(\Phi) = [\boldsymbol{\Gamma}^T \otimes \boldsymbol{\Omega}] \text{Vec}(\mathbf{A}). \quad (14)$$

The result provided by the algebraic interpolation is the generic matrix of coefficients \mathbf{A} , which is given by

$$\text{Vec}(\mathbf{A}) = [\boldsymbol{\Gamma}^T \otimes \boldsymbol{\Omega}]^\dagger \text{Vec}(\Phi), \quad (15)$$

where : $\text{Vec}(\mathbf{A}) = [a_{11} \dots a_{n1} \dots a_{n2} \dots a_{np}]^T$.

Once the matrices \mathbf{A}_r and \mathbf{A}_z are known, the MDR, such as $\psi(z, y) : (z, y) \rightarrow (\Phi_{ij})$, is solved for any point within the domain $\mathcal{G}' = \{(r, z) \in [0, L]\}$.

Given the calibration matrices \mathbf{A}_r and \mathbf{A}_z , and the orthogonal basis $\boldsymbol{\omega}(r)$ and $\boldsymbol{\gamma}(z)$, the system of equation expressed in (11) and (12) is completely determined. By differentiating $\boldsymbol{\omega}(r)$ and $\boldsymbol{\gamma}(z)$ in ∂r and ∂z , respectively, we can obtain the complete formulation of the MIR in (2). The following system of equations – expressed for the single solution $[\Phi_r, \Phi_z]^T$ – provides the ground to derive the Jacobian:

$$\begin{cases} \Phi_r = \boldsymbol{\omega}(r) \mathbf{A}_r \boldsymbol{\gamma}(z) \\ \Phi_z = \boldsymbol{\omega}(r) \mathbf{A}_z \boldsymbol{\gamma}(z) \end{cases} \quad (16)$$

Applying (2) to this system of equations, and deriving the partial derivatives of $\Phi = [\Phi_r, \Phi_z]^T$ such as $\frac{\partial \Phi_r}{\partial r}$, $\frac{\partial \Phi_r}{\partial z}$, $\frac{\partial \Phi_z}{\partial r}$, $\frac{\partial \Phi_z}{\partial z}$, the gradient of Φ becomes

$$\nabla \Phi = \begin{cases} \nabla \Phi_r = \frac{\partial(\boldsymbol{\omega}(r) \mathbf{A}_r \boldsymbol{\gamma}(z))}{\partial r} + \frac{\partial(\boldsymbol{\omega}(r) \mathbf{A}_r \boldsymbol{\gamma}(z))}{\partial z} \\ \nabla \Phi_z = \frac{\partial(\boldsymbol{\omega}(r) \mathbf{A}_z \boldsymbol{\gamma}(z))}{\partial r} + \frac{\partial(\boldsymbol{\omega}(r) \mathbf{A}_z \boldsymbol{\gamma}(z))}{\partial z} \end{cases} \quad (17)$$

Considering that the derivatives of the constant coefficient matrices \mathbf{A}_r and \mathbf{A}_z are null, as well as $\frac{\partial \boldsymbol{\omega}(r)}{\partial z}$ and $\frac{\partial \boldsymbol{\gamma}(z)}{\partial r}$, (17) simplifies to:

$$\begin{aligned} \frac{\partial \Phi_r}{\partial r} &= \frac{\partial \boldsymbol{\omega}(r)}{\partial r} \mathbf{A}_r \boldsymbol{\gamma}(z) \\ \frac{\partial \Phi_r}{\partial z} &= \boldsymbol{\omega}(r) \mathbf{A}_r \frac{\partial \boldsymbol{\gamma}(z)}{\partial z} \\ \frac{\partial \Phi_z}{\partial r} &= \frac{\partial \boldsymbol{\omega}(r)}{\partial r} \mathbf{A}_z \boldsymbol{\gamma}(z) \\ \frac{\partial \Phi_z}{\partial z} &= \boldsymbol{\omega}(r) \mathbf{A}_z \frac{\partial \boldsymbol{\gamma}(z)}{\partial z} \end{aligned} \quad (18)$$

In order to obtain the expression of $\frac{\partial \boldsymbol{\omega}(r)}{\partial r}$ and $\frac{\partial \boldsymbol{\gamma}(z)}{\partial z}$, a derivation is applied to the vectors constituting the orthogonal basis $\boldsymbol{\omega}(r), \boldsymbol{\gamma}(z)$. This leads to the following expression for the Jacobian \mathbf{J}_Φ :

$$\mathbf{J}_\Phi = \nabla_{\bar{\mathbf{p}}_c} \Phi(r, z) = \begin{bmatrix} \frac{\partial \Phi_r}{\partial r} & \frac{\partial \Phi_r}{\partial z} \\ \frac{\partial \Phi_z}{\partial r} & \frac{\partial \Phi_z}{\partial z} \end{bmatrix} \quad (19)$$

Therefore, the magnetic field vector incremental difference $\Delta \mathbf{B}_i = [\Delta B_r, \Delta B_z]_i^T$ is given by

$$\Delta \mathbf{B}_i = \begin{bmatrix} \Delta B_r \\ \Delta B_z \end{bmatrix}_i = \mathbf{J}_\Phi \Delta \mathbf{p}_{ci} \quad (20)$$

This result can be used in (3) to estimate the magnetic field \mathbf{B}_{i+1} by continuously updating $\Delta \mathbf{B}_i$ to the current magnetic field value:

$$\mathbf{B}_{i+1} = \mathbf{B}_i + \Delta \mathbf{B}_i = \mathbf{B}_i + \mathbf{J}_\Phi \Delta \mathbf{p}_{ci}. \quad (21)$$

In conclusion, the following equation shows the iterative method to localize the WCE, estimating the current position $\mathbf{p}_{ci+1} = [r_{i+1}, z_{i+1}]^T$ of the capsule as

$$\mathbf{p}_{ci+1} = \mathbf{p}_{ci} + \Delta \mathbf{p}_{ci} = \mathbf{p}_{ci} + \mathbf{J}_{\Phi}^{-1} \Delta \mathbf{B}_i, \quad (22)$$

where \mathbf{J}^{-1} is the pseudo-inverse of the Jacobian, which applies the least squares method of optimization to the solution [23]. The term $\Delta \mathbf{B}_i$ is the difference in magnetic field recorded from the previous measurement.

C. Three Dimensional Reconstruction

In order to track the WCE by applying the iterative algorithm, both the spatial orientation of the capsule and the external magnetic source pose must be known with respect to a common reference frame. The magnetic field vector \mathbf{B}_c at the capsule position $\tilde{\mathbf{p}}_c$ – expressed in the capsule frame $[\hat{\mathbf{x}}_c, \hat{\mathbf{y}}_c, \hat{\mathbf{z}}_c]$ – is measured by the onboard sensors. This vector can be expressed in the EPM frame $[\hat{\mathbf{x}}, \hat{\mathbf{y}}, \hat{\mathbf{z}}]$ by applying the geometrical transformation \mathbf{R}_c^{EPM} , thus obtaining \mathbf{B} .

Then, considering Figs. 1 and 3, the magnetic field vector \mathbf{B} is expressed in cylindrical coordinates from its cartesian coordinates, such as: $\mathbf{B} = [B_x, B_y, B_z]^T \rightarrow [B_r, B_z]^T$ and θ , where θ correspond to the azimuthal coordinate of the capsule position $\tilde{\mathbf{p}}_c$. The relationships that transform the magnetic field vector $\mathbf{B}_c = [B_x \hat{\mathbf{x}}, B_y \hat{\mathbf{y}}, B_z \hat{\mathbf{z}}]$ from cartesian to cylindrical coordinates are:

$$\begin{aligned} B_r &= \sqrt{(B_x \hat{\mathbf{x}})^2 + (B_y \hat{\mathbf{y}})^2} \hat{\mathbf{r}} \\ B_z &= B_z \hat{\mathbf{z}} \\ \theta &= \text{atan2}(B_y, B_x) \hat{\theta} \end{aligned} \quad (23)$$

where B_x, B_y, B_z are the cartesian components of the magnetic field vector \mathbf{B} with respect to the EPM frame $[\hat{\mathbf{x}}, \hat{\mathbf{y}}, \hat{\mathbf{z}}]$. The axial and radial magnetic field components can be fed into the iterative algorithm, which derives the radial and axial coordinates of the capsule $\mathbf{p}_c = [p_r, p_z]$. These can be used in combination with θ to derive the three cartesian coordinates as follows:

$$\begin{aligned} p_x &= p_r \cos(\theta) \hat{\mathbf{x}} \\ p_y &= p_r \sin(\theta) \hat{\mathbf{y}} \\ p_z &= p_z \hat{\mathbf{z}} \end{aligned} \quad (24)$$

III. CAPSULE ORIENTATION ALGORITHM

This section presents the algorithm used to detect the change in capsule orientation and to generate the rotational matrix \mathbf{R}_c with respect to the global frame. This algorithm based on the fusion of inclinometer and gyroscope outputs is widely adopted in literature and is provided here for the sake of completeness. The capsule orientation knowledge is required in our magnetic localization approach in order to express the magnetic field vector \mathbf{B}_c in the EPM frame.

Referring to Fig. 1, the accelerometer can be used as an inclinometer to obtain the absolute values of the two orientational angles α and β [24]. The rotations about \mathbf{x}_c and \mathbf{y}_c are derived directly from the gravitational vector \mathbf{g}

projection mapped on the three orthogonal axes of the onboard accelerometer as

$$\begin{aligned} \alpha &= \text{atan2}(a_y, \sqrt{a_x^2 + a_z^2}) \\ \beta &= \text{atan2}(a_x, \sqrt{a_y^2 + a_z^2}) \end{aligned} \quad (25)$$

where a_x, a_y, a_z are the three accelerometer outputs.

A number of methods for inertial navigation can be adopted to estimate the third orientation angle γ , which is the rotational angle along the gravitational vector \mathbf{g} . Examples span from fusing gyroscope and inclinometer measurements [25, 26] to applying a quaternion-based algorithm to inertial data [27]. The approach we have adopted involves applying the axis-angle method for rotational matrices to the gyroscope outputs [28]. Briefly, it is possible to extract the rotation γ about the global axis \mathbf{z}_w by building the rotational matrix $\Delta \mathbf{R}_c$ with respect to the moving frame attached to the capsule $[\hat{\mathbf{x}}_c, \hat{\mathbf{y}}_c, \hat{\mathbf{z}}_c]$. The instantaneous variations in capsule orientation can be derived from the gyroscope outputs as

$$\Delta \alpha_c = g_x \Delta t \quad \Delta \beta_c = g_y \Delta t \quad \Delta \gamma_c = g_z \Delta t \quad (26)$$

where $\Delta[\alpha_c, \beta_c, \gamma_c]$ are the instantaneous angle variations at the capsule moving frame within a measurement loop that lasts Δt . The instantaneous capsule rotational matrix $\Delta \mathbf{R}_c$ is then defined as

$$\Delta \mathbf{R}_c = \mathbf{R}_x(\Delta \alpha_c) \mathbf{R}_y(\Delta \beta_c) \mathbf{R}_z(\Delta \gamma_c) \quad (27)$$

where $\mathbf{R}_x, \mathbf{R}_y, \mathbf{R}_z$ are the rotational matrixes with respect to the $\mathbf{x}_c, \mathbf{y}_c$, and \mathbf{z}_c axis, respectively. Then, the axial-angle representation of the rotational matrix $\Delta \mathbf{R}_c$ is derived, thus achieving the angle of rotation θ and the axis of rotation ω :

$$\begin{aligned} \theta &= \arccos\left(\frac{\text{trace}(\Delta \mathbf{R}_c) - 1}{2}\right) \\ \omega &= \frac{1}{2 \sin(\theta)} \sum_{j=1}^3 (\hat{\mathbf{e}}_{c_j, i} \times \hat{\mathbf{e}}_{c_j, i+1}) \end{aligned} \quad (28)$$

where $\hat{\mathbf{e}}_{c_j, i}$ and $\hat{\mathbf{e}}_{c_j, i+1}$ are the unit vectors of the capsule frame at the i -th and $(i+1)$ -th iterations, respectively. Finally, the axis-angle representation θ, ω must be reoriented according to the capsule orientation with respect to the global frame at the previous time step, \mathbf{R}_c^{t-1} . The third coordinate of the axial-angle representation corresponds to the capsule angle variation $\Delta \gamma$ about $\hat{\mathbf{z}}_w$. The capsule absolute orientation γ about the global axis $\hat{\mathbf{z}}_w$ is achieved by summation of $\Delta \gamma$ at each loop.

IV. SIMULATION-BASED VALIDATION

The proposed approach was validated using a NdFeB cylindrical EPM with an axial N52-grade magnetization, a diameter of 5 cm, and a length of 5 cm. The size L of the squared domain \mathcal{G}' was fixed at 15 cm. The reference values for the magnetic field in \mathcal{G}' were obtained using Comsol Multiphysics, using a pitch of 0.2 mm for the mesh. The mathematical analysis and simulations were performed by using MATLAB, MathWorks Inc.

A. Magnetic Direct Relationship

Comsol Multiphysics was also used to create the 15×15 matrix Φ_r and the 18×18 matrix Φ_z relative to the radial and axial components of the magnetic field, respectively. These two matrices were interpolated using two vectors of modal basis functions ω and γ . The vector ω captures variations of the magnetic field as a function of radial distance r and it is given by:

$$\omega(r) = \left[1/2, \cos\left(\frac{\pi r}{L}\right), \sin\left(\frac{\pi r}{L}\right), \dots, \cos\left(\frac{\pi 12r}{L}\right), \sin\left(\frac{\pi 12r}{L}\right), r, r^2, \dots, r^5 \right] \quad (29)$$

Similarly, the dependence of the magnetic field on variations of the axial component z is captured by $\gamma(z)$:

$$\gamma(z) = \left[1/2, \cos\left(\frac{\pi z}{L}\right), \sin\left(\frac{\pi z}{L}\right), \dots, \cos\left(\frac{\pi 12z}{L}\right), \sin\left(\frac{\pi 12z}{L}\right), z, z^2, \dots, z^5 \right] \quad (30)$$

The modal basis functions were chosen based on simulation of the approximation residue with the minimum number of terms that provide a relative error of less than 10% within a portion of at least 70% of the domain \mathcal{G}' .

Both \mathbf{A}_r and \mathbf{A}_z were derived applying (15), thus obtaining 31×31 matrices. The interpolation was obtained by applying (11) and (12) to any radial and axial coordinate of the domain \mathcal{G}' . The interpolation error was evaluated by comparing the interpolated magnetic field with the reference values derived by Comsol Multiphysics. Given the position vector $\mathbf{p}_{ci} = [r, z]_i^T$ within \mathcal{G}' , Fig. 4-a shows the module of the relative error for the radial magnetic field component, while Fig. 4-b shows the module of the relative error for the axial component. Table I reports the portions of \mathcal{G}' where the interpolation error is below 1%, 5%, 10%, and 20% for both the axial and the radial component of the magnetic field. The radial component estimation presents a relative error below 10% for the 86% of the radial magnetic field map. The axial component estimation shows that the 70% of the axial magnetic field map presents a relative error below 10%. Whenever the value of magnetic field intensity is very small, or null, a small approximation noise leads to a high relative error, as it is shown in Fig. 4. These results show an efficient estimation of both B_r and B_z , thus allowing the MDR to be analytically derived via (16).

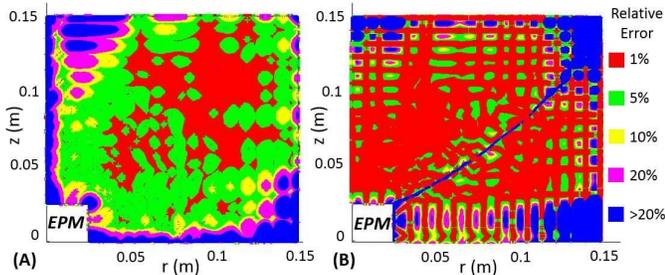


Fig. 4. Relative error for the radial (A) and axial (B) magnetic field estimated by the MDR within \mathcal{G}' .

Fig. 5 shows the ratio of the relative error of the single dipole model [29] to the relative error of our interpolation

method, where the relative error is calculated with respect to the reference values derived by Comsol Multiphysics. The blue regions –ratio between 0 and 1– of the maps correspond to a similar or better performance of interpolation for the dipole model comparing with the proposed method. The dark red regions correspond to ratio greater than 8. Table I reports the portions of \mathcal{G}' where the interpolation error of the dipole model is below 1%, 5%, 10%, and 20% for both the axial and the radial component of the magnetic field. From these results, we can conclude that the proposed approach provides a more accurate approximation for the magnetic field in both components.

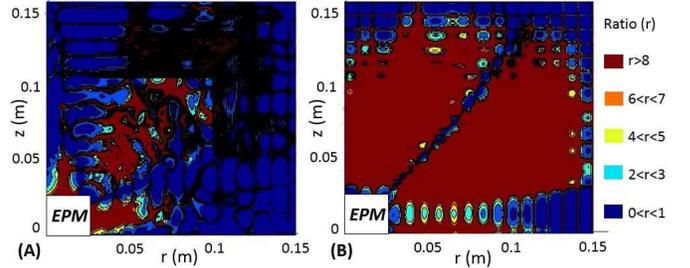


Fig. 5. The ratio of relative errors of the single dipole model to the interpolation model for the radial (A) and axial (B) magnetic field components. Black regions stem from visualization artifacts due to oscillations in the ratio from 3 to 8 times.

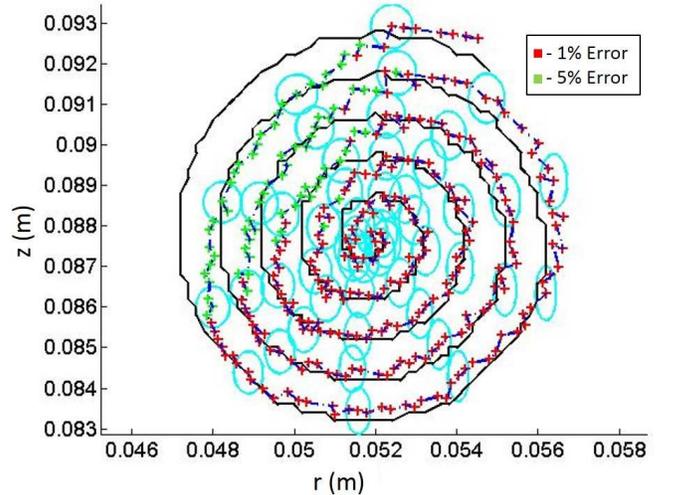


Fig. 6. Simulated motion of a capsule along a spiral trajectory in the center of \mathcal{G}' . The black line represents the reference trajectory, while the crossed line shows the capsule position estimated by applying the Jacobian-based iterative method. The cyan ellipses represent the ellipsoid of localization uncertainty due to magnetic field sensor noise. Colors in the crossed line express the relative error in position detection for the radial component.

B. Magnetic Inverse Relationship

The pose detection iterative method based on (22) was assessed by simulating the capsule motion along a spiral path, starting from a central position in the map $\mathbf{p}_c \approx [0.09, 0.055]m$, reaching a final diameter of 1 cm, and assuming the orientation given. Fig. 6 shows the reference trajectory

TABLE I

PORTIONS OF \mathcal{G}' SHOWING DIFFERENT LEVELS OF RELATIVE ERROR IN THE INTERPOLATED MAGNETIC FIELD FROM THE PROPOSED METHOD AND THE SINGLE MAGNETIC DIPOLE MODEL.

Level of relative error	Radial Component	Axial Component
Below 1%	42%	30%
Below 5%	78%	61%
Below 10%	86%	70%
Below 20%	92%	79%
Magnetic dipole model	Radial Component	Axial Component
Below 1%	12%	0.4%
Below 5%	63%	2%
Below 10%	81%	5%
Below 20%	90%	10%

and its pose estimation. The color map represents the relative error of the radial coordinate. The estimation of the simulated capsule pose results in an axial coordinate relative error below 1%, with respect to its current position, for almost the entire simulation. The radial coordinate relative error is below 1% for the upper-right, lower-left and lower-right quadrants of the spiral path represented in Fig. 6. The upper-left quadrant presents a relative error below 5%. This increased error is related to the radial localization error map of Fig. 4.A. Since the center of the spiral is at the upper left quadrant of Fig. 4.A, where the radial error increases with proximity to the top left corner, the error of localization along the spiral exhibits a similar trend. Also, considering the noise of magnetic field sensor readings, the outcome of the localization algorithm for each capsule position is represented by an ellipsoid of uncertainty (in cyan in Fig. 6). In this simulation, we used the noise levels of ± 0.08 mT and ± 0.05 mT in measuring B_r and B_z based on experimental characterization from the platform described in Section V-A. This simulation demonstrates an average sub-millimeter localization accuracy for both the radial and axial component.

V. EXPERIMENTAL ASSESSMENT

A. Experimental Platform

1) *Hardware*: The experimental platform, represented in Fig. 7.A, is composed of the WCE, the EPM, a robotic manipulator (RM), and a personal computer (PC) connected to a wireless transceiver via the universal serial bus (USB) port. The real-time algorithm runs on the PC and communicates with the capsule through a USB transceiver. The EPM is an NdFeB (magnetization N52, magnetic remanence 1.48 T) cylindrical permanent magnet with axial magnetization. The EPM diameter and length are both equal to 50 mm, while the mass is 772 g. A six-DOF robot (RV6SDL, Mitsubishi Corp., Japan) mounts at its end-effector the EPM. The robot is controlled in real time through a multi-thread C++ software application, which is described in section V-A3. The manipulator is used to control and track the EPM position and orientation with respect to the global reference frame $[\hat{x}_w, \hat{y}_w, \hat{z}_w]$, which is assumed to be superimposed on the manipulator ground frame $[\hat{x}_0, \hat{y}_0, \hat{z}_0]$. The current EPM pose for the localization algorithm is derived from the robot end-effector pose, which is available at the application interface

level with a resolution of 2×10^{-2} mm in position and 1×10^{-3} degree in orientation. The EPM orientation frame $[\hat{x}, \hat{y}, \hat{z}]$ is an input for the localization algorithm (as described in section II-C), while the EPM pose, as acquired by the robot encoders, is used as a reference position for the experimental assessment. A load cell (MINI 45, ATI Industrial Automation, USA), mounted in between the EPM and the RM, allows the EPM to be moved via admittance control for the general assessment described in Section V-B5.

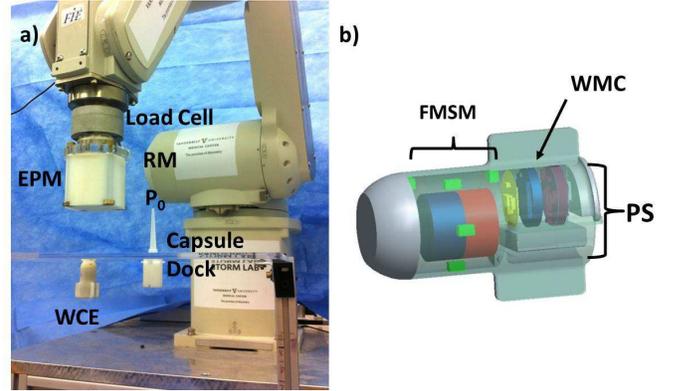


Fig. 7. Experimental platform: a) Robotic Manipulator (RM) and External Permanent Magnet (EPM). b) Visual rendering of the Wireless Capsule Endoscope (WCE) and its internal components, where FMSM is the Force and Motion Sensing Module, WMC is the Wireless MicroController and PS is the Power Supply.

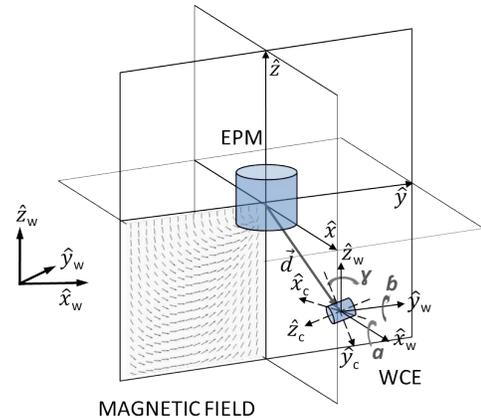


Fig. 8. Schematic representation of the global frame, EPM frame and capsule frame. The capsule orientation angles $[\alpha, \beta, \gamma]$ are shown with respect to the global frame.

2) *Wireless Capsule*: The WCE, schematically represented in Fig. 7.B, hosts the Force and Motion Sensing Module (FMSM), which was presented in [4], Wireless MicroController (WMC), and Power Supply (PS). The outer shell is fabricated in VeroWhite 3D printer material (OBJET 30, Stratasys, USA). The current prototype is 36 mm in length, 17.5 mm in diameter, and 15 g in mass. The capsule shell has four lateral wings that are used as a reference to achieve a precise alignment for the capsule frame $[\hat{x}_c, \hat{y}_c, \hat{z}_c]$ during the calibration.

The FMSM is composed of six Magnetic Field Sensors (MFS, A1391, Allegro MicroSystems, USA), an Inertial Mea-

surement Unit (IMU) embedding both an accelerometer and a gyroscope (LSM 330, STMicroelectronics, Switzerland), and an off-the-shelf NdFeB (N52) cylindrical magnet, which was axially magnetized with 1.48 T of magnetic remanence, 11 mm in diameter and 11 mm in height. The readings of the magnetic sensors integrated in the FMSM are acquired by the onboard 16-bit Analog to Digital Converter (ADC, AD7689, Analog Devices, Inc. USA). An acquisition cycle starts from sampling six analog inputs connected to the MFS outputs. Then, the six digitized values of acceleration and angular speed are received from the IMU. This dataset is acquired every 4.4 ms by the WMC (CC2530, Texas Instruments, USA) and used to build a 36-byte package together with the capsule status indicators (i.e., battery level, start/stop bytes). This package is then transmitted by the WMC to the external transceiver over a 2.4 GHz carrier frequency, with a refresh time of 6 ms (wireless data throughput 42.4 kbit/s), resulting in a sampling rate of 166 Hz. The external transceiver is based on an identical WMC which communicates with the PC through a USB-serial converter (UM232R, FTDI, UK).

The power supply module embeds a low-dropout voltage regulator (LDO) (TPS73xx, Texas Instruments, USA) to provide a stable supply to both the FMSM and the communication module. In order to limit the current consumption when the device is not acquiring measurements, a digital output of the microcontroller can drive the SLEEP pin of all the MFS. This results in a current consumption which varies between 400 mA, when the microcontroller is in low power mode, and 20 mA when it is in IDLE mode with the radio active. Average current consumption rises to 48 mA during a single cycle of sensor data acquisition and wireless transmission. The power source used is a 50 mAh, 3.7 V rechargeable LiPo battery (Shenzhen Hondark Electronics Co., Ltd., China).

3) *Software Architecture*: A multi-thread C++ WIN32 application running on the PC unbundles the data and shares them with three other parallel threads. The first thread controls the robotic manipulator through a UDP/IP communication with a refresh rate of 140 Hz. It sends the desired pose to the robot controller and then receives the robot pose feedback. The second thread implements a digital Kalman filter for each of the six MFS and the six IMU outputs before running the iterative localization algorithm. The algorithm outputs the 6-DOF capsule pose estimation $\mathbf{p} = [x, y, z, \alpha, \beta, \gamma]$ with respect to the EPM frame $[\hat{x}, \hat{y}, \hat{z}]$. The third thread manages a TCP/IP communication with a MATLAB application (Mathworks, USA), which displays the localization algorithm estimation. The data transfer rate for the robot controller applications is 83 Hz. The refresh time for the capsule pose estimation \mathbf{p} and the capsule wireless data transfer is 6.8 ms (refresh rate 150 Hz). Referring to Fig. 8, the MATLAB application displays the capsule position and orientation $\mathbf{p} = [x, y, z, \alpha, \beta, \gamma]$ with respect to the EPM reference frame $[\hat{x}, \hat{y}, \hat{z}]$ in real time (refresh every 30 ms) on a 3D plot. Current pose numerical values are also displayed.

B. Experiments and Results

1) *Capsule orientation algorithm assessment*: Because the localization method we propose also relies on real-time cap-

sule orientation data, the first step in the experimental assessment consisted in validating the algorithm described in section III. In order to quantify the absolute error in capsule orientation, the WCE was rigidly attached to the end effector of the RM. The orientation of the WCE was varied within a range of $\pm 90^\circ$ about each of the three axes $[x_{EPM}, y_{EPM}, z_{EPM}]$ by adopting combined motions for a total of one minute. Inertial data acquired by the WCE were sent over the wireless link, while the orientation of the end effector, as measured by the RM built-in encoders, was adopted as a reference. The average orientation error was $3.4^\circ \pm 3.2^\circ$ for α , $3.7^\circ \pm 3.5^\circ$ for β , and $3.6^\circ \pm 2.6^\circ$ for γ .

A second experiment aimed to quantify the steady-state drift for the capsule orientation algorithm. This is particularly relevant for the estimation of γ , which, unlike α and β , is obtained by iterative integration. For this test, the WCE was locked into the capsule dock (see Fig. 7 or the multimedia attachment 1) for 7.5 minutes while acquiring data and running the capsule orientation algorithm. The average error and its standard deviation over the entire period was $0.34^\circ \pm 0.18^\circ$ for α , $0.27^\circ \pm 0.17^\circ$ for β , and $1.8^\circ \pm 1.1^\circ$ for γ , while the absolute error at the end of the 7.5 minutes was 0.5° for α , 0.2° for β , and 5.2° for γ .

2) *Steady state positional drift evaluation*: This set of experiments, referred to as T01, was aimed at evaluating the localization algorithm behavior in steady conditions. Before the trials began, the iterative localization algorithm was initialized as shown in the multimedia attachment 1. The calibration consisted of three steps. First, the capsule was placed into the capsule dock, with a known position and orientation with respect to the global frame $[x_w, y_w, z_w]$. Then, the magnetic field sensors in the WCE were biased while maintaining the EPM outside the workspace. Finally, the EPM was moved to a reference position with respect to the WCE, and the relative distance between the EPM and the WCE, as derived by design, was used to initialize $\mathbf{p}(t = 0)$ (digitization phase in the multimedia attachment 1).

After the initial calibration, the EPM was moved to eight different positions within the workspace, while the WCE was maintained in the capsule dock. Each position was chosen to be at about 10 cm from the center of the workspace along both the radial and axial coordinate. The radial and axial coordinates of the EPM were fixed to 80 mm and 130 mm, respectively. The azimuth coordinate θ_{EPM} was changed from zero to 2π in $\pi/4$ steps. Each EPM position was maintained for one minute, while recording the localization data. The results were compared to the reference EPM pose as derived by the RM encoders. Table II reports the azimuth coordinate, the average radial error and the average axial error for each of the eight EPM positions.

For each trial, the relative error, the drift, and the residual measurement noise were statistically analysed while the system was not subjected to relative motion between the WCE and the EPM. The proposed localization method presented an average absolute and relative error for the radial component of $2.9 \pm 1.4\text{mm}$ and $1.85 \pm 2.1\%$, respectively. The average absolute and relative errors for the axial component were $2.1 \pm 1.0\text{mm}$ and $1.9 \pm 0.9\%$, respectively.

TABLE II
RESULTS OF THE STEADY STATE POSITIONAL DRIFT EXPERIMENT (T01).

$\theta_{EPM} (^{\circ})$	T01-RE (mm)	T01-AR (mm)
0	0.3 ± 0.3	1.5 ± 0.5
45	1.5 ± 0.9	0.3 ± 0.3
90	7.2 ± 2.8	6.4 ± 3.3
135	4.4 ± 2.1	3.4 ± 1.6
180	0.5 ± 0.5	1.8 ± 0.8
225	5.1 ± 2.8	2.5 ± 1.2
270	3.7 ± 1.5	0.6 ± 0.2
315	0.5 ± 0.4	0.4 ± 0.3

Typical trends for radial and axial component estimation are shown in Fig. 9. During the trials, the pose estimation presented a drift due to the system noise and the iterative integration. However, the relative error was always below 5%. The residual measurement noise (Fig. 9.d) had a gaussian distribution (Jarque-Bera normality test with h equal to 1 and p-value 0.1) with null average and a bandwidth below 0.5%, which remained constant for the entire duration of each trial. The magnetic field measurement noise fused with the IMU measurements did not affect the localization algorithm, thus resulting in a stable long-term behavior.

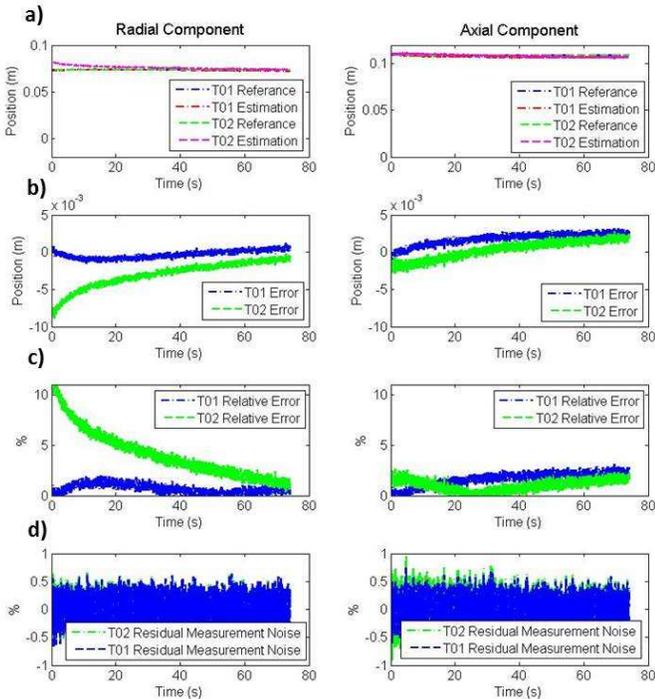


Fig. 9. Results for the steady state positional drift experiment (T01) and for the initialization error evaluation (T02) with an initialization error of 10mm. Both T01 and T02 results are evaluated for the radial (left column) and the axial (right column) component. (a) Reference position vs. estimation. (b) Absolute positional errors. (c) Relative positional errors. (d) Residual measurement noise. The azimuth error is presented in Fig. 12.

3) *Robustness to initialization errors*: This set of experiments, referred to as T02, was aimed at assessing the algorithm sensitivity to errors in position initialization. These trials were performed by moving the EPM to the same eight positions used for T01, while maintaining the WCE fixed into the capsule dock. For each EPM position, four different tests were performed by adding an increasing error e to the initialization

distance $\mathbf{p}(t = 0)$ as measured during calibration. In particular, the error e had a random direction in \hat{r} and \hat{z} and an increasing module (i.e., 1 mm, 5 mm, 10 mm, and 20 mm). As in T01, each test was one minute long.

Considering all 32 tests performed, the average absolute and relative error for the radial component were $15.5 \pm 4.2mm$ and $19.5 \pm 6.0\%$, respectively. The axial component had an average absolute error of $13.6 \pm 3.9mm$ and an average relative error of $12.1 \pm 3.5\%$.

Typical trends for radial and axial component estimation affected by a 10 mm error in position initialization are shown in Fig. 9. In this case, the absolute and the relative error (Fig. 9.b and Fig. 9.c, respectively) decreased within the duration of the trial, never exceeding 10% of the reference value. Interestingly, the localization algorithm was able to correct the initialization error with time. The residual measurement noise for both the radial and the axial component (Fig. 9.d) presented the same behavior observed in T01 trials.

4) *Robustness to positional lag*: This set of trials aimed at evaluating the effect that a lag between the EPM and the WCE may have on the localization algorithm. In particular, our goal was to quantify the minimum value for the relative speed between the EPM and the WCE that would prevent the localization algorithm to converge. For reference, the typical endoscope absolute speed during a colonoscopy is in the order of 0.8 mm/s to 1.6 mm/s [30]. However, for magnetic capsule endoscopy, the relative EPM-WCE speed is ideally null, as the WCE should be following the EPM motion under the effect of magnetic coupling. This is true as long as the WCE is able to freely move inside the lumen.

After the initial calibration as described for T01, five trials were performed by moving the EPM at increasing speeds while collecting localization data. Like the previous experiments, the WCE was locked into the capsule dock. The EPM was initially positioned at 110 mm along the radial component and 110 mm along the axial component, and then moved by 200 mm along y_w at a constant acceleration. For the five trials, acceleration was set to 0.396, 0.793, 1.190, 1.587, and 1.984 $\frac{m}{s^2}$, respectively. The multimedia extension 1 shows one of these trials, while the results for the experiment with 1.984 $\frac{m}{s^2}$ acceleration are reported in Fig. 10. As expected, the EPM motion along y_w only affected the radial component of the localization algorithm, leaving the axial component almost unperturbed.

For this set of trials, the localization algorithm presented a relative error in the radial component of 10% for a relative speed of $0.221 \pm 0.046 \frac{m}{s}$. This increased up to 20% for a relative speed of $0.335 \pm 0.050 \frac{m}{s}$. The average absolute error in the radial component was $11.86 \pm 8.36mm$, with an average relative error of $16.3 \pm 10.2\%$. For the axial component, the average absolute error was $2.66 \pm 1.8mm$, with an average relative error of $2.3 \pm 1.6\%$.

Given these results, we can conclude that the algorithm is sensitive to the relative speed between the WCE and the EPM and the relative error exceeds 10% if the relative speed is greater than $0.2 \frac{m}{s}$. As previously discussed, this speed is well above the values that we expect to experience during magnetic manipulation of a WCE.

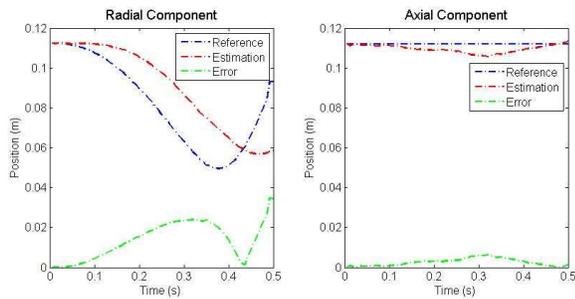


Fig. 10. Position estimation results during the positional lag trial with uniform acceleration of $1.984 \frac{m}{s^2}$.

5) *General assessment:* The final experiment aimed at validating the localization algorithm for a generic trajectory of the EPM, with the WCE fixed into the capsule dock. After calibration, the EPM was moved via admittance control to form a three-dimensional loop within the workspace, starting from the initialization position $\mathbf{p}(t=0)$. During this trial, the EPM coordinates spanned from about -10 cm to 10 cm along both \hat{x}_w and \hat{y}_w axes, and from 6 cm to 12 cm away from the WCE position along the \hat{z}_w axis.

For the entire trajectory, the proposed method of localization presented an average absolute error in the radial component of $6.2 \pm 4.4 \text{ mm}$ and an average relative error of $5.7 \pm 7.6\%$. The average absolute error for the axial component was $6.9 \pm 3.9 \text{ mm}$, with an average relative error of $7.0 \pm 4.9\%$. The average absolute error for the azimuth component (θ) was $5.4^\circ \pm 7.9^\circ$.

The trajectory (as reconstructed from the RM encoders) and its estimation are represented in Fig. 11. Typical trends for the radial (r), the axial (z), and the azimuthal (θ) component estimations are shown in Fig. 12.a,c,e, while the absolute and relative errors are reported in Fig. 12.b,d,f. The azimuthal component presents a large absolute error when the radial component of the capsule position is approaching zero. This is due to minor misalignments between the capsule and the EPM. This error is significantly attenuated in the conversion of the pose from cylindrical to Cartesian coordinates by applying (24), as the radial component p_r is very small or equal to zero.

It is worth noting that the experimental assessment showed an error that is about one order of magnitude larger than what was observed by simulation. This is probably due to the noise introduced by the sensors and by the digitization process.

Real-time operation of the localization algorithm for random motion of the WCE is shown in the multimedia extension 2. On the left side of the screen, the localization output is plotted in real-time showing the WCE and the EPM reference frames.

In the multimedia extension 3, the localization is performed while moving the EPM parallel to a plexiglass pipe placed at an angle with respect to the global frame. In this case, the WCE is free to move in the pipe under the effect of magnetic coupling. The distance between the EPM and the WCE is about 10 cm . The localization real-time output $\mathbf{p} = [x, y, z, \alpha, \beta, \gamma]$ and the EPM position are both superimposed to the video stream. This demonstrates the ability of the proposed localization algorithm to track the WCE in real-time

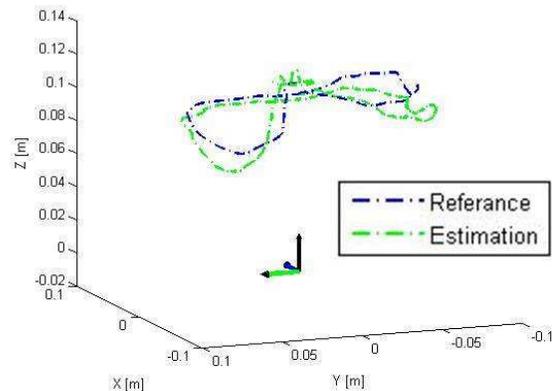


Fig. 11. Three-dimensional representation of the EPM trajectory and its estimation by the localization algorithm.

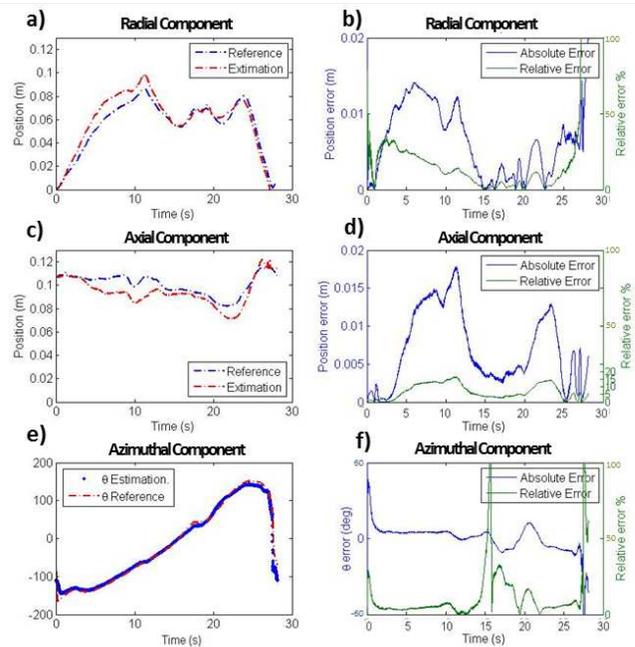


Fig. 12. Typical trends for the radial (a), the axial (c) and the azimuth (e) component during the final experiment, and related absolute and relative errors (b, d, and f, respectively).

during magnetic manipulation.

VI. CONCLUSIONS

This paper was motivated by the limitations of existing magnetic localization algorithms in terms of computational time, precision, and compatibility with magnetic manipulation of endoscopic capsules. To overcome these limitations, we put forward a new method for real-time localization using fusion of inertial data with information from magnetic field sensors, combined with an iterative Jacobian-based approach. Our strategy uniquely applies a parametrization of the magnetic field using least squares interpolation over an exact finite element solution, thus overcoming the limitations of the simplistic dipole model. To achieve this parametrization, we

used Kronecker products and a modal fitting to describe the magnetic field. To assist with real-time localization (which is paramount for solving a nonlinear inverse problem), we used the Jacobian of the magnetic field intensity relative to pose perturbations of the endoscopic capsule. This allowed the use of a local linearization approach that is similar to the resolved rates method for inverse kinematics of serial robots.

Our algorithm was evaluated by simulation and experiments. We investigated the robustness of our pose estimates of the wireless capsule to initialization errors. We also characterized the residual measurement noise and the effect of positional lag when the magnet driving the capsule was moving. Our results showed that, even though the proposed algorithm exhibits limitations of convergence for fast relative motions, the pose estimation of the magnetic capsule for clinically realistic speeds was effective and reliable. In particular, experimental results showed an average error (expressed in cylindrical coordinates) below 7 mm in both the radial and axial components, and 5° in the azimuthal component. The average errors for the capsule orientation angles, obtained by fusing gyroscope and inclinometer measurements, were 0.3° for α and β , and 5° for γ . Overall, the relative error always remained below 10%. The proposed localization algorithm was able to run at a 1 ms refresh rate, an order of magnitude below what was reported in previous works. The overall refresh rate, including sensor data acquisition and wireless communication, was 7 ms, thus enabling closed-loop control strategies for WCE magnetic manipulation running faster than 100 Hz. Since the least square interpolation present some regions of the magnetic field domain \mathcal{G}' where the relative error is greater than 20%, in future applications the robot path planner can be instructed to follow the capsule and to enclose it in an optimal localization area to avoid these regions.

Drift – a common problem in integrative methods – may become an issue over time and affect the precision of localization. A possible solution is to integrate the proposed approach with absolute localization strategies [3, 4] or with techniques fusing multiple sensor data having different resolutions and refresh rates, as proposed in [31, 32, 33] for SLAM applications. Since the final goal is to localize the capsule during magnetic manipulation, the behaviour of the algorithm must be quantitatively assessed with the capsule in motion against a reference localization method (i.e., vision-based localization as in [2]), exploiting also inertial navigation system theory by applying the extended Kalman filter [34, 35].

In summary, the proposed localization strategy is compatible with magnetic manipulation of WCE, does not require clear line-of-sight, has a resolution that is finer than the capsule size, and a refresh rate that is adequate for real-time closed loop robotic control. This represents an enabling technology that can move us toward intelligent control of a WCE during an endoscopic procedure.

REFERENCES

- [1] P. Valdastrì, M. Simi, and R. J. Webster III, “Advanced technologies for gastrointestinal endoscopy,” *Annual Review of Biomedical Engineering*, vol. 14, pp. 397–429, 2012.
- [2] A. W. Mahoney and J. J. Abbott, “Five-degree-of-freedom manipulation of an untethered magnetic device in fluid using a single permanent magnet with application in stomach capsule endoscopy,” *The International Journal of Robotics Research*, 2015, in press, available on-line.
- [3] C. Di Natali, M. Beccani, and P. Valdastrì, “Real-time pose detection for magnetic medical devices,” *IEEE Trans. Magn.*, vol. 49, no. 7, pp. 3524–3527, 2013.
- [4] C. Di Natali, M. Beccani, K. Obstein, and P. Valdastrì, “A wireless platform for in vivo measurement of resistance properties of the gastrointestinal tract,” *Physiological measurement*, vol. 35, no. 7, p. 1197, 2014.
- [5] T. D. Than, G. Alici, H. Zhou, and W. Li, “A Review of Localization Systems for Robotic Endoscopic Capsules,” *IEEE Trans. Bio-Med. Eng.*, vol. 59, no. 9, pp. 2387–2399, 2012.
- [6] C. Hu, M. Li, S. Song, R. Zhang, M.-H. Meng *et al.*, “A cubic 3-axis magnetic sensor array for wirelessly tracking magnet position and orientation,” *Sensors Journal, IEEE*, vol. 10, no. 5, pp. 903–913, 2010.
- [7] S. Song, B. Li, W. Qiao, C. Hu, H. Ren, H. Yu, Q. Zhang, M. Q.-H. Meng, and G. Xu, “6-d magnetic localization and orientation method for an annular magnet based on a closed-form analytical model,” *Magnetics, IEEE Transactions on*, vol. 50, no. 9, pp. 1–11, 2014.
- [8] D. M. Pham and S. M. Aziz, “A real-time localization system for an endoscopic capsule,” in *Intelligent Sensors, Sensor Networks and Information Processing (ISSNIP), 2014 IEEE Ninth International Conference on*. IEEE, 2014, pp. 1–6.
- [9] K. M. Popek, A. W. Mahoney, and J. J. Abbott, “Localization method for a magnetic capsule endoscope propelled by a rotating magnetic dipole field,” in *Robotics and Automation (ICRA), 2013 IEEE International Conference on*. IEEE, 2013, pp. 5348–5353.
- [10] S. Yim and M. Sitti, “3-d localization method for a magnetically actuated soft capsule endoscope and its applications,” *Robotics, IEEE Transactions on*, vol. 29, no. 5, pp. 1139–1151, 2013.
- [11] M. Salerno, R. Rizzo, E. Sinibaldi, and A. Menciassi, “Force calculation for localized magnetic driven capsule endoscopes,” in *Robotics and Automation (ICRA), 2013 IEEE International Conference on*, 2013, pp. 5354–5359.
- [12] D. Whitney, “Resolved Motion Rate Control of Manipulators and Human Prostheses,” *IEEE Transactions on Man Machine Systems*, vol. 10, no. 2, pp. 47–53, Jun. 1969.
- [13] J. Nocedal and S. J. Wright, *Numerical Optimization*, T. V. Mikosch, S. M. Robinson, and S. Resnick, Eds. Springer, 2006.
- [14] E. P. Furlani, *Permanent Magnet and Electromechanical Devices*. Elsevier, 2001, pp. 131–135.
- [15] —, *Permanent magnet and electromechanical devices [electronic resource]: materials, analysis, and applications*. Access Online via Elsevier, 2001.
- [16] E. Furlani and M. Knewton, “A three-dimensional field solution for permanent-magnet axial-field motors,” *Mag-*

- netics, *IEEE Transactions on*, vol. 33, no. 3, pp. 2322–2325, 1997.
- [17] G. S. Chirikjian and J. W. Burdick, “A Modal Approach to Hyper-Redundant Manipulator Kinematics,” *IEEE Transactions on Robotics and Automation*, vol. 10, no. 3, pp. 343–354, 1994.
- [18] J. Zhang, K. Xu, N. Simaan, and S. Manolidis, “A pilot study of robot-assisted cochlear implant surgery using steerable electrode arrays,” in *Medical Image Computing and Computer-Assisted Intervention—MICCAI 2006*. Springer, 2006, pp. 33–40.
- [19] J. Zhang, J. T. Roland, S. Manolidis, and N. Simaan, “Optimal path planning for robotic insertion of steerable electrode arrays in cochlear implant surgery,” *Journal of medical devices*, vol. 3, no. 1, 2009.
- [20] H. F. Davis, *Fourier series and orthogonal functions*. DoverPublications. com, 1963.
- [21] N. Csanyi and C. K. Toth, “Some aspects of using Fourier analysis to support surface modeling,” in *Proceedings of Pecora 16, Global Priorities in Land Remote Sensing*, Sioux Falls, South Dakota, October 2005, pp. 1–12.
- [22] J. Brewer, “Kronecker products and matrix calculus in system theory,” *Circuits and Systems, IEEE Transactions on*, vol. 25, no. 9, pp. 772–781, 1978.
- [23] P. Lancaster and Miron Tismensky, *The Theory of Matrices*, 2nd ed. Academic Press, 1985.
- [24] F. C. A. Devices, “Using an accelerometer for inclination sensing,” *Application note AN-1057*, 2011.
- [25] H. J. Luinge, P. H. Veltink, and C. T. Baten, “Estimating orientation with gyroscopes and accelerometers,” *Technology and health care*, vol. 7, no. 6, pp. 455–459, 1999.
- [26] M. Ignagni, “Optimal strapdown attitude integration algorithms,” *Journal of Guidance, Control, and Dynamics*, vol. 13, no. 2, pp. 363–369, 1990.
- [27] J. Favre, B. Jolles, O. Siegrist, and K. Aminian, “Quaternion-based fusion of gyroscopes and accelerometers to improve 3d angle measurement,” *Electronics Letters*, vol. 42, no. 11, pp. 612–614, 2006.
- [28] Y. Nakamura, *Advanced Robotics: Redundancy and Optimization*, 1st ed. Boston, MA, USA: Addison-Wesley Longman Publishing Co., Inc., 1990.
- [29] J. C. Springmann, J. W. Cutler, and H. Bahcivan, “Magnetic sensor calibration and residual dipole characterization for application to nanosatellites,” in *Proceedings of the AIAA/AAS Astrodynamics Specialist Conference*, Toronto, Canada, August 2010, pp. 1–14.
- [30] P. Valdastri, R. J. Webster III, C. Quaglia, M. Quirini, A. Menciassi, and P. Dario, “A new mechanism for mesoscale legged locomotion in compliant tubular environments,” *IEEE Trans. Robot.*, vol. 25, no. 5, pp. 1047–1057, 2009.
- [31] M. Kaess, H. Johannsson, R. Roberts, V. Ila, J. J. Leonard, and F. Dellaert, “isam2: Incremental smoothing and mapping using the bayes tree,” *The International Journal of Robotics Research*, p. 0278364911430419, 2011.
- [32] V. Indelman, S. Williams, M. Kaess, and F. Dellaert, “Factor graph based incremental smoothing in inertial navigation systems,” in *Information Fusion (FUSION), 2012 15th International Conference on*. IEEE, 2012, pp. 2154–2161.
- [33] L. Carlone, R. Aragues, J. A. Castellanos, and B. Bona, “A fast and accurate approximation for planar pose graph optimization,” *The International Journal of Robotics Research*, p. 0278364914523689, 2014.
- [34] M. S. Grewal, L. R. Weill, and A. P. Andrews, *Global positioning systems, inertial navigation, and integration*. John Wiley & Sons, 2007.
- [35] B. Barshan and H. F. Durrant-Whyte, “Inertial navigation systems for mobile robots,” *Robotics and Automation, IEEE Transactions on*, vol. 11, no. 3, pp. 328–342, 1995.



Christian Di Natali (S'10) received B.S. and M.S. degrees (Hons.) in Biomedical Engineering from the University of Pisa, in 2008 and 2010. In 2011, he joined the Institute of BioRobotics of Scuola Superiore Sant'Anna (SSSA), Pisa, Italy, as Research Assistant. In 2015, he graduated with a PhD in Mechanical Engineering from Vanderbilt University, Nashville, TN, where he was actively involved in the design of advanced magnetic coupling for surgery and endoscopy, controlled mechatronic platforms and magnetic localization.



Marco Beccani (S'11) received a Master's degree in Electronic Engineering from the University of Pisa, Pisa, Italy, in 2010. In 2015, he graduated with a PhD in Mechanical Engineering from Vanderbilt University, Nashville, TN. He is currently a post-doctoral fellow at University of Pennsylvania, Philadelphia, PA.



Nabil Simaan (SM 04) received his Ph.D. in mechanical engineering from the Technion: Israel Institute of Technology, Haifa, Israel, in 2002. In 2005, he joined Columbia University, New York, NY, as an Assistant Professor. In 2009 he received the NSF Career award to design new algorithms and robots for safe interaction with the anatomy. He was promoted to Associate Professor in 2010 and subsequently he joined Vanderbilt University, Nashville, TN in Fall 2010.



Pietro Valdastri (M'05, SM'13) received a Master's (Hons.) degree in Electronic Engineering from the University of Pisa, Italy, in 2002, and a Ph.D. degree in Biomedical Engineering from SSSA, Pisa, Italy. He is Assistant Professor in the Department of Mechanical Engineering at Vanderbilt University and Director of the STORM Lab. In 2015, he received the NSF Career award to study and design capsule robots for medical applications.