



Deposited via The University of Leeds.

White Rose Research Online URL for this paper:

<https://eprints.whiterose.ac.uk/id/eprint/114557/>

Version: Accepted Version

Proceedings Paper:

Miao, Q, Lo, HS, Xie, SQ et al. (2017) Iterative learning control method for improving the effectiveness of upper limb rehabilitation. In: 2016 23rd International Conference on Mechatronics and Machine Vision in Practice (M2VIP). 23rd International Conference on Mechatronics and Machine Vision in Practice, 28-30 Nov 2016, Nanjing, Jiangsu, China. IEEE. ISBN: 9781509027644.

<https://doi.org/10.1109/M2VIP.2016.7827302>

© 2016, IEEE. This is an author produced version of a paper published in 2016 23rd International Conference on Mechatronics and Machine Vision in Practice (M2VIP). Personal use of this material is permitted. Permission from IEEE must be obtained for all other users, including reprinting/ republishing this material for advertising or promotional purposes, creating new collective works for resale or redistribution to servers or lists, or reuse of any copyrighted components of this work in other works. Uploaded in accordance with the publisher's self-archiving policy.

Reuse

Items deposited in White Rose Research Online are protected by copyright, with all rights reserved unless indicated otherwise. They may be downloaded and/or printed for private study, or other acts as permitted by national copyright laws. The publisher or other rights holders may allow further reproduction and re-use of the full text version. This is indicated by the licence information on the White Rose Research Online record for the item.

Takedown

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing eprints@whiterose.ac.uk including the URL of the record and the reason for the withdrawal request.

Iterative Learning Control Method for Improving the Effectiveness of Upper Limb Rehabilitation

QING MIAO

Mechanical and Electrical Engineering
Wuhan University of Technology
Wuhan, Hubei Province, China
miaoqing0702@126.com

Sheng Quan. Xie

Mechanical Engineering
University of Auckland
Auckland, New Zealand
s.xie@auckland.ac.nz

Ho Shing Lo

Mechanical Engineering
University of Auckland
Auckland, New Zealand
hlo015@aucklanduni.ac.nz

Hong Sheng LI

Mechanical and Electrical Engineering
Wuhan University of Technology
Wuhan, Hubei Province, China
lihswh@gmail.com

Abstract—In rehabilitation, passive control mode is common used at early stages of the post-stroke therapy, when the impaired limb is usually unresponsive. The simplest is the use of a proportional-integral-derivative (PID) feedback control which usually regulates the position or the interaction force along a known reference. Nonetheless PID method cannot achieve an ideal tracking performance due to dynamical uncertainties and unknown time-varying periodic disturbances from the environment. In order to minimize steady-state error with respect to uncertainties in exoskeleton passive control, Iterative Learning Control(ILC) and Neural PID control are proposed to improve the control effective of conventional linear PID. In this paper, two different control algorithms are introduced. Moreover, an experimental study on a 5-DOF upper limb exoskeleton with them is addressed for comparison.

Keywords—upper limb exoskeleton; passive control mode; Iterative Learning Control (ILC); Neural PID Introduction

I. INTRODUCTION

According to World Health Organization (WHO), stroke is the third most common cause of death in developed countries, exceeded only by coronary heart disease and cancer [1]. Conventionally, stroke rehabilitation needs one-to-one manual interactions with therapists [7]. Treatment plans mean that it should therapy for several weeks, which makes it difficult to offer highly intensive treatment for patients [10]. In recent years, using rehabilitation robot has been received increasing attention for stroke recovery [5], which can provide repetitive, task-specific and effective treatment of the impaired upper limb [10].

In rehabilitation, it is hardy for patients to move their impaired upper limbs that are very unresponsive at the beginning [5]. Thus, passive training could be a feasible way in early period [11]. Thus, passive control has been to proposed [16], which means to control the motion of an exoskeleton rigidly along a desired reference trajectory through position

feedback control with high corrective gains [6]. Actually, passive control can adopt various techniques to achieve. Proportional-integral-derivative (PID) feedback control is the most common method [3]. It is usually regulates the interaction force or the position or along a known reference (e.g. a trajectory or a force field model), and also used either at the joint or at the end-effector level. Nevertheless, there are few research regarding PID gains tuning for upper limb robots. Independently using PID tuning algorithms is not possible due to the responses being nonlinear. Therefore, intelligent control strategies have been researched and widely used [2, 26, 28]. Neural PID is a typical one. Being similar with robust adaptive control methods [24, 29], it could adjust weights in order to adjust parameters of PID by updating laws to make the closed-loop systems stable. Iterative Learning Control (ILC) has been important to provide improvement in tracking performance compared with the use of feedback controllers alone [19]. Initially, ILC algorithms were developed based on the contraction mapping theory and required priori knowledge [20]

In this paper, two different passive control methods were proposed for passive trajectory tracking of an upper limb exoskeleton robot in order to improve its effectiveness when treating stroke patients. The effectiveness of the proposed adaptation strategy is evaluated by experiments. The paper is organized as follows: Section II, iterative learning control and neural PID control are introduced, and back propagation neural network (BPNN) algorithm was presented for PID parameters adjusting. A 5 DOF upper limb exoskeleton is presented and experiments are carried out in Section III. Section IV gives conclusions of this work.

II. METHODS

A. Iterative Learning Control (ILC)

Fig 1 shows the ILC Control Structure [23]. UP represents the upper limb robot; C is the feedback of the controller,

and L is the feed-forward of the controllers; MEM is the memory for the system; the control law $u = u_k + u_c$, which $k = 1, 2, \dots, N$ is the current iteration number, where the feed-forward u_k is the input trajectory; q_k is the real output trajectory; and q_d is the desired output trajectory. u_{k+1} is next term of u_k , which presents the feed-forward off-lined calculated iteration result. The feed-forward controller is based on the update control law that improves the feed-forward control term (u_k). For the nonlinear dynamic model, we propose the following update control law[19]:

$$u_{k+1}(t) = u_k(t) + \Gamma \dot{e}_k(t) + \Phi e_k(t) + \Psi \int_0^t e_k(\tau) d\tau \quad (1)$$

where Γ, Φ, Ψ are learning gain matrixes; the error between real position and the desired position is $e_k(t) = q_d(t) - q_k(t)$; the

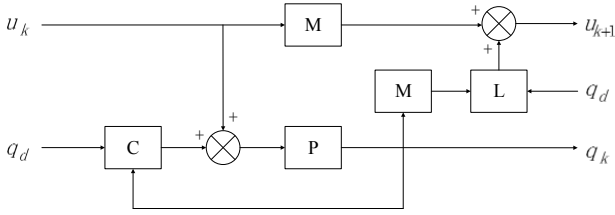


Fig. 1 ILC Control Structure

initial input of feed-forward control is $u_0(t)$; $t : t \in [0, T]$ is the tracking time, and $[0, T]$ is the robot tracking time interval.

Learning algorithm convergence analysis is very important for ILC. An adequate condition called spectral radius method is a good way to measure whether proposed update control law could guarantee robustness and convergence. It has been proved the considered dynamic model of the upper limb robot if it can be satisfied as followed [18]:

$$\|I - LA^{-1}\| \leq \rho < 1 \quad (2)$$

where I is the identity matrix, A is the inertia matrix of the dynamic equations of motion, L is the learning operator that is to be specified, and $\|\cdot\|$ is the Euclidean matrix norm.

B. Neural PID Control

Neural PID control method is to adjust the weights of each neural network in order to achieve optimal PID parameters by training[27]. Back propagation neural network (BPNN) structure has been used. Where, $\tilde{x}_m = x_m - x_d$, $\tilde{\dot{x}}_m = \dot{x}_m - \dot{x}_d$, $\tilde{\ddot{x}}_m = \ddot{x}_m - \ddot{x}_d$. There are two inputs and three outputs for the controller. First one is the i th error of position and $e_{ip} = P_{id} - P_i$ second one is the i th error of velocity $\dot{e}_{ip} = \dot{P}_{id} - \dot{P}_i$. Outputs are the i th desired PID parameters K_{ip}, K_{li} and K_{ld} .

This neural network included two inputs, four hidden neurons and three output neurons.

$$i_n = e(n), n = 1, 2 \quad (3)$$

$$net_{hm}(k) = \sum_{n=1}^2 \omega_{hmn} i_n, m = 1, 2, \dots, 4 \quad (4)$$

$$O_{hm}(k) = f(net_{hm}(k)), m = 1, 2, \dots, 4 \quad (5)$$

$$O(z) = f(z) = \frac{1}{1 + e^{(-z)}} \quad (6)$$

where i_n are inputs, which $e_{ip} = e(1)$ and $\dot{e}_{ip} = e(2)$, net_{hm} is the input of the m th hidden layer, The variable ω_{hmn} denotes the weight between neurons m and n . Then use the logistic function to squash (8) in order to get the output of $O(z)$ is in general non-linear and differentiable so that it is commonly used as a logistic function. Correspondingly, it could be calculated both inputs and outputs of output layer.

$$net_{ov}(k) = \sum_{v=1}^3 \omega_{ovm} o_{hm}, m = 1, 2, \dots, 4 \quad (7)$$

$$O_{ov}(k) = f(net_{ov}(k)), v = 1, 2, 3 \quad (8)$$

The squared error function can be used to achieve the error for each output neuron and sum them to get the total error

$$E_{o1}(k) = \frac{1}{2} (K_{ip}(k) - K_{ip}(k))^2 \quad (9)$$

$$E_{o2}(k) = \frac{1}{2} (K_{li}(k) - K_{li}(k))^2 \quad (10)$$

$$E_{o3}(k) = \frac{1}{2} (K_{ld}(k) - K_{ld}(k))^2 \quad (11)$$

$$E_{total}(k) = E_{o1}(k) + E_{o2}(k) + E_{o3}(k) \quad (12)$$

Where $K_{ip}(k)$, $K_{li}(k)$ and $K_{ld}(k)$ are the training target PID parameters, which are compared with real outputs $K_{ip}(k)$, $K_{li}(k)$ and $K_{ld}(k)$. The goal is to update each of the weights in the network so that they cause the actual outputs to be closer the target outputs, thereby minimizing the error for each output neuron and the network as a whole.

$$\Delta\omega(k) = \eta \frac{\partial E_o(k)}{\partial \omega} + \gamma \Delta\omega(k-1) \quad (13)$$

With gradient descent method, learning rate η and inertia coefficient γ can be used to describe weights changing.

III. EXPERIMENT AND RESULTS

In order to test these two passive control methods, a 5DOF exoskeleton has been used to track trajectory experiments. The exoskeleton consists of 5 DOF, including actuating 4 DOF (3 DOF for shoulder joint spherical motion and 1 DOF for actuating and elbow 1 DOF (Fig.3). In addition, the exoskeleton could achieve flexion & extension, for both shoulder and elbow, medial & lateral rotation running and abduction & adduction

for shoulder. By using the exoskeleton, the patients should be in a seated position in order to ensure the patients will be limited in the appropriate usage position. The exoskeleton uses five motors to operate the exoskeleton to ensure they do not interfere with the movements of the exoskeleton. A keyed shaft transmits torque between the motors and the link segments[16].

The Newton-Euler method is used to derive the equations of motion for each exoskeleton joint (14) where τ_a is the actuation torque produced by the motor-gearbox unit, τ_i is the torque due to inertia, τ_g is the torque caused by gravitational forces, τ_f is the friction torque, τ_d is the torque caused by the disturbance user's limb movements. On a flip side, torque caused by coriolis and centrifugal effects are small since the exoskeleton operates at low velocities and are assumed to be negligible.

$$\tau_a = \tau_i + \tau_g + \tau_f + \tau_d \quad (14)$$

The inertial torque experienced by an exoskeleton joint is given by (15) where I_s is the inertia tensor of the segment at the joint coordinate system, α is the angular acceleration of the joint and N is the total number of segments acting on the joint.

$$\tau_i = \sum_S^N I_s \times \alpha \quad (15)$$

As with inertial torque, the torque caused by gravitational effects also depends on the configuration of the exoskeleton. The gravitational torque acting on an exoskeleton joint is given by (16) where p_s is the displacement vector from the joint to the center of mass of segment, m_s is the mass of the segment, R_s is the rotation transformation matrix between the global coordinate system and the joint coordinate system and g is the gravitational constant vector in the global coordinate system.

$$\tau_g = \sum_S^N p_s \times (m_s (R_s g)) \quad (16)$$

Friction is a resistance to joint motion and is present in the motor, gearbox, bearings and the Joint 4 rail. In the present work, friction is modeled using a piecewise function (17) where k_f is the positive torque constant determined experimentally. The friction torque is assumed to act in the direction opposite to joint motion and if the joint is stationary then the friction torque is considered to be acting opposite to the direction of the control output.

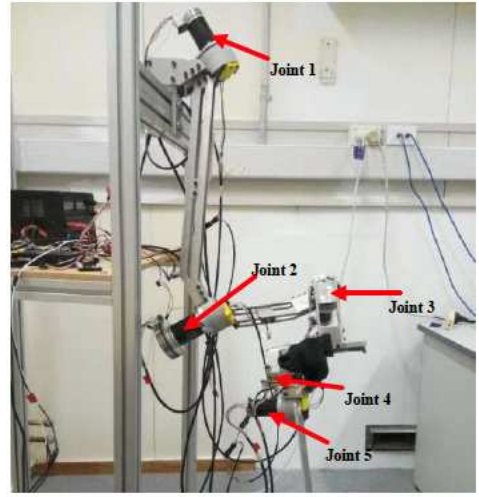


Fig. 2 The 5 DOF exoskeleton prototype

$$\tau_f \begin{cases} k_f & \text{if } (\dot{\theta} < 0 \text{ or } \dot{\theta} = 0 \wedge \tau_m < 0) \\ 0 & \text{if } (\dot{\theta} = 0) \dots \tau_m = 0 \\ -k_f & \text{if } (\dot{\theta} > 0 \text{ or } \dot{\theta} = 0 \wedge \tau_m > 0) \end{cases} \quad (17)$$

The experiments consist of 2 parts. Firstly, it is designed to use elbow joint to track a $\pi/4$ arc trajectory in order to test the transient response of two methods. Secondly, a round-trip repetitive $\pi/4$ arc trajectory is used to test rapidity, accuracy and stability. For contrasting intuitively, linear PID control is implemented. It regards angle error as the result, and uses Root-Mean-Square Error (RMSE) to measure the property.

The control result of first test is shown in Fig.3, and the RMSE is shown in Table I. The performances (main transient) of both Neural PID and ILC methods are good, but linear PID one is poorer. There still exists regulation error because of mechanical vibration. Moreover, it is shown in Table I that the errors of Neural PID are smaller than ILC ones.

The control result of second test is shown in Fig.5, and the RMSE is shown in Table II, the performances of ILC method is much better than Neural PID method, According to Table II, it shows that ILC method has the smaller errors.

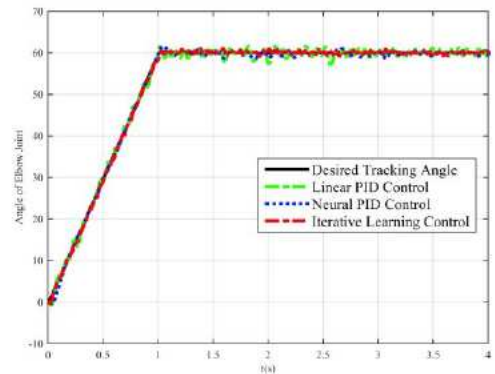


Fig. 3 Elbow Angle in first test

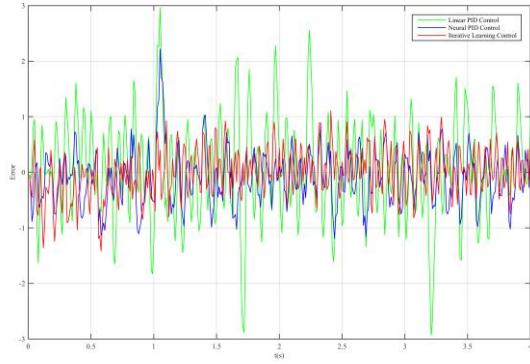


Fig. 4 Elbow Angle Errors in first test

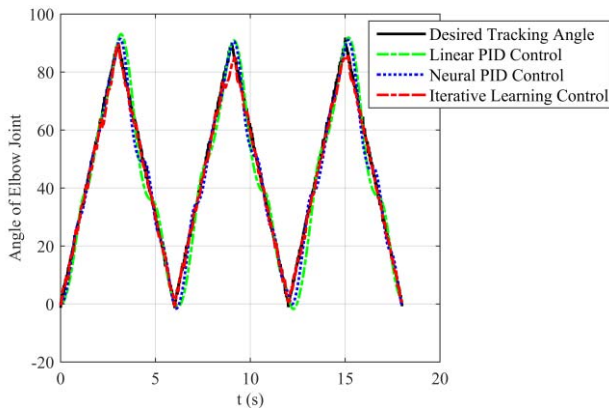


Fig. 5 Elbow Angle Errors in second test

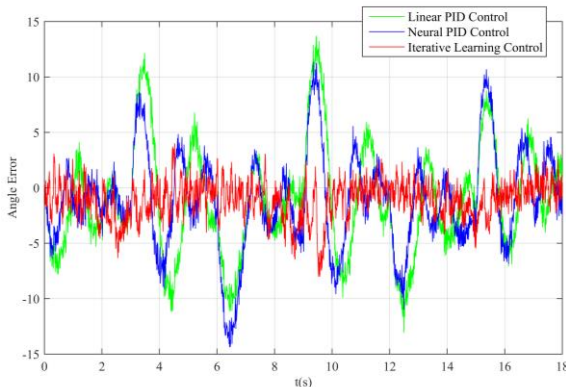


Fig. 6 Elbow Angle Errors in second test

Clearly, both Neural PID control and ILC could successfully achieve a good performance of tracking trajectory. Because they have compensator to handle the uncertainties, instead of using fixed PID parameters. Neural PID has good performance of the transient response due to its previous training parameters. However, ILC has advantage improving effectiveness by learning laws

TABLE I RMSE of first test

	ILC	Neural PID	Linear PID
RMSE	1.44	1.75	2.92
	1.75	1.81	2.76
	0.44	0.96	2.44
	0.07	0.39	2.37
	0.19	0.29	1.92

TABLE II RMSE of second test

	ILC	Neural PID	Linear PID
RMSE	5.50	9.44	10.90
	3.50	7.45	9.84
	2.41	7.43	9.88
	4.48	8.43	11.90
	1.88	6.91	9.81

IV. CONCLUSION

The paper proposed a new ILC method and neural PID control method for improving the effectiveness of upper limb rehabilitation. The control methods have been developed for a passive control mode of an upper limb exoskeleton, which was developed at the Medical and Rehabilitation Robotics group at the University of Auckland. The neural PID and ILC have been developed to control the 5-DOF exoskeleton robot. Theory and experiment analysis show the different characteristics and reliable validity of control methods in the passive control mode. Neural PID method is an available control strategy displacing linear PID by achieving training parameters, the method has been compared with ILC method. Evidences showed that the ILC method is an effective technique for repetitive rehabilitation passive training because of its learning ability, which will increase tracking accuracy.

ACKNOWLEDGMENT

The authors would like to acknowledge the funding support from the Lottery Health Research Council of New Zealand and the scholarship from the Chinese Scholarship Council.

REFERENCES

- [1] "World health organization website," Mar. 2013.
- [2] Ho Shing Lo, Sheng Quan Xie, Exoskeleton robots for upper-limb rehabilitation: State of the art and future prospects, *Medical Engineering & Physics*, vol. 34 p. 261–268, 2012
- [3] R. W. Teasell and L. Kalra, "What's New in Stroke Rehabilitation," *Stroke*, vol. 35, pp. 383-385, 2004.
- [4] J.Alvarez-Ramirez, R.Kelly, I.Cervantes, Semiglobal stability of saturated linear PID control for robot manipulators, *Automatica*, vol.39,989-995, 2003
- [5] V. S. Huang and J. W. Krakauer, "Robotic neurorehabilitation: A computational motor learning perspective," *Journal of NeuroEngineering and Rehabilitation*, vol. 6, 2009.

- [6] Tommaso Proietti; Vincent Crocher; Agnes Roby-Brami; Nathanael Jarrasse, "Upper-limb robotic exoskeletons for neurorehabilitation: a review on control strategies", IEEE Reviews in Biomedical Engineering, vol: PP, Issue: 99, 2016
- [7] G. Kwakkel, B. Kollen, and H. Krebs, "Effects of robot-assisted therapy on upper limb recovery after stroke: a systematic review," NNR, 2007.
- [8] Wen Yu and Jacob Rosen, A Novel Linear PID Controller for an Upper Limb Exoskeleton, 49th IEEE Conference on Decision and Control, CDC'10, Atlanta, USA, 3548-3553, 2010.
- [9] L. Marchal-Crespo and D. Reinkensmeyer, "Review of control strategies for robotic movement training after neurologic injury," JNER, vol. 6, no. 1, p. 20, 2009.
- [10] V. Klamroth-Marganska, J. Blanco, K. Campen, A. Curt, V. Dietz, T. Ettlin, M. Felder, B. Fellinghauer, M. Guidali, and A. Kollmar, "Three-dimensional, task-specific robot therapy of the arm after stroke: a multicentre, parallel-group randomised trial," Lancet Neurol, vol. 13, no. 2, pp. 159–166, 2014.
- [11] K. Kong and D Jeon, "Fuzzy control of a new tendon-driven exoskeletal power assistive device", in Proc. IEEE/ASME International Conference on Advanced Intelligent Mechatronics, Monterey ,California, 2005, pp. 146-151.
- [12] Krebs, H.I., Palazzolo, J.J., Dipietro, L., Ferraro, M., Krol, J., Ranekleiv, K., Volpe, B.T., Hogan, N.: Rehabilitation robotics: Performance-based progressive robot-assisted therapy. *Auton. Robots* 15(1), 7–20 (2003).
- [13] T. Ando, M. Watanabe, and M. G. Fujie, "Extraction of voluntary movement for an EMG controlled exoskeletal robot of tremor patients," in International IEEE/EMBS Conference on Neural Engineering, 2009, pp. 120-123.
- [14] P. K. Artemiadis and K. J. Kyriakopoulos, "Estimating arm motion and force using EMG signals: On the control of exoskeletons," in IEEE/RSJ International Conference on Intelligent Robots and Systems, 2008, pp. 279-284.
- [15] "Development and control of a wearable robot for rehabilitation of elbow and shoulder joint movements," in IECON, pp. 1506–1511, IEEE, 2010.
- [16] H. Lo and S. Xie, "An upper limb exoskeleton with an optimized 4r spherical wrist mechanism for the shoulder joint," in AIM, pp. 269–274, IEEE, 2014
- [17] A. Frisoli, C. Procopio, C. Chisari, I. Creatini, L. Bonfiglio, M. Bergamasco, B. Rossi, M. Carboncini, et al., "Positive effects of robotic exoskeleton training of upper limb reaching movements after stroke," JNER, vol. 9, no. 1, p. 36, 2012
- [18] M. Milot, S. Spencer, V. Chan, J. Allington, J. Klein, C. Chou, J. Bobrow, S. Cramer, and D. Reinkensmeyer, "A crossover pilot study evaluating the functional outcomes of two different types of robotic movement training in chronic stroke survivors using the arm exoskeleton bones," JNER, vol. 10, p. 112, Dec. 2013.
- [19] Gopinath S, Kar I. Iterative learning control scheme for manipulators including actuator dynamics. *Mechanism and Machine Theory* 2004; 39:1367–1384.
- [20] Xu JX. Analysis of iterative learning control for a class of nonlinear discrete-time systems. *Automatica* 1997; 33(10):1905–1907.
- [21] Delchev K, Zahariev E. Computer simulation based synthesis of learning control law of robots. *Mechanics Based Design of Structures and Machines* 2008; 36(3):225–248.
- [22] Delchev K. Iterative learning control for nonlinear systems: a bounded-error algorithm. *Asian Journal of Control* 2013; 15(2):453–460.
- [23] C.T. Freemana, A.-M. Hughesb, J.H. Burrigeb, P.H. Chappella, P.L. Lewina, E. Rogersa, Iterative learning control of FES applied to the upper extremity for rehabilitation, *Control Engineering Practice*, vol 17, p 368–381.
- [24] P.Rocco, Stability of PID control for industrial robot arms, *IEEE Transactions on Robotics and Automation*, VOL.12, NO. 4 , 606-614,1996
- [25] T.Dierks, S.Jagannathan, Neural Network Output Feedback Control of Robot Formations, *IEEE Transactions on Systems, Man, and Cybernetics, Part B*, Vol.40, No.4, 383-399, 2010
- [26] C-S.Chen, Dynamic Structure Neural-Fuzzy Networks for Robust Adaptive Control of Robot Manipulators, *IEEE Trans. Industrial Electronics*, VOL. 55, NO. 9, 3402-3414, 2008
- [27] G.M. Scott, J. W.Shavlik, W. H. Ray, Refining PID Controllers Using Neural Networks, *Neural Computation*, Vol. 4, No. 5, 746-757, 1992
- [28] Xie, S. Q. and Jamwal, P., "An Iterative Fuzzy Controller for Pneumatic Muscle Driven Robot", *Expert Systems with Applications*, available online at, <http://dx.doi.org/10.1016/j.eswa.2010.12.154>, 38 (7), pp. 8128-8137, 2011.
- [29] Graham, A. E., Young, A. J., Xie, S. Q., 2007, "Rapid Tuning of Controllers by IFT for Profile Cutting Machines", *Mechatronics*, Vol.17, No.2-3, pp.121~128, 2007
- [30] Liang Zhou, Wei Meng, Charles Z. Lu, Quan Liu, Qingsong Ai and Sheng Q. Xie, "Bio-Inspired Design and Iterative Feedback Tuning Control of a Wearable Ankle Rehabilitation Robot", *ASME Journal of Computing and Information Science in Engineering*, published online June 17, 2016. doi:10.1115/1.4033900