



Deposited via The University of Sheffield.

White Rose Research Online URL for this paper:

<https://eprints.whiterose.ac.uk/id/eprint/117693/>

Version: Accepted Version

Article:

Roberts, C.M., Olivier, N., Wardley, W.P. et al. (2016) Interscale mixing microscopy: far-field imaging beyond the diffraction limit. *Optica*, 3 (8). pp. 803-808.

<https://doi.org/10.1364/OPTICA.3.000803>

Reuse

Items deposited in White Rose Research Online are protected by copyright, with all rights reserved unless indicated otherwise. They may be downloaded and/or printed for private study, or other acts as permitted by national copyright laws. The publisher or other rights holders may allow further reproduction and re-use of the full text version. This is indicated by the licence information on the White Rose Research Online record for the item.

Takedown

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing eprints@whiterose.ac.uk including the URL of the record and the reason for the withdrawal request.

Interscale Mixing Microscopy: far field imaging beyond the diffraction limit

CHRISTOPHER M. ROBERTS,^{1,*} NICOLAS OLIVIER,² WILLIAM P. WARDLEY,²
 SANDEEP INAMPUDI,^{1,&} WAYNE DICKSON,² ANATOLY V. ZAYATS,² VIKTOR A.
 PODOLSKIY¹

¹Department of Physics and Applied Physics, University of Massachusetts Lowell, Lowell, MA 01854

²Department of Physics, King's College London, Strand, London WC2R 2LS, United Kingdom

[&]Present address: ECE Department, Northeastern University, Boston, MA, 02115

*Corresponding author: Christopher_Roberts@student.uml.edu

Received XX Month XXXX; revised XX Month, XXXX; accepted XX Month XXXX; posted XX Month XXXX (Doc. ID XXXXX); published XX Month XXXX

Optical microscopy is widely used to analyze the properties of materials and structures, to identify and classify these structures, as well as to understand and control their response to external stimuli. The extent of available applications is determined largely by the resolution offered by a particular microscopy technique. Here we present an analytic description and an experimental realization of interscale mixing microscopy, a diffraction-based imaging technique that is capable of detecting and characterizing wavelength/10 objects in far-field measurements with both coherent and incoherent broadband light. This technique is aimed at analyzing subwavelength objects based on far-field measurements of the interference created by the objects and a finite diffraction grating. A single measurement, analyzing the multiple diffraction orders, is often sufficient to determine the parameters of the object. The presented formalism opens the door for spectroscopy of nanoscale objects in the far-field.

OCIS codes: (180.0180) Microscopy, (050.1950) Diffraction gratings, (110.3010) Image reconstruction techniques

<http://dx.doi.org/10.1364/optica.99.099999>

1. Introduction

The detection and visualization of sub-wavelength objects has numerous applications in imaging, spectroscopy, material science, biology, healthcare, and security. In conventional optical microscopy, the fundamental resolution limit is often associated with diffraction criteria by Rayleigh and Abbe [1,2]. According to these criteria, the smallest feature one can optically resolve is approximately limited to $(\lambda_0/2NA)$ with λ_0 being vacuum wavelength and NA being numerical aperture of the objective [3] (Fig.1). In practical terms, however, the position of an isolated object can be determined with much better accuracy; and recent methods which rely on the control of a molecule's fluorescent state have used the fluorescence property to achieve imaging with nanometer resolution [4,5,6]. However, these methods — as well as other optical super-resolution techniques [7] — are limited to the study of fluorescent objects. In recent years, several label-free optical imaging techniques relying on first-order diffraction and multiple measurements to access high-spatial frequency components of the object have been demonstrated, such as structured illumination microscopy (SIM) [8], optical diffraction tomography (ODT) [9,10], or the far field superlens (FSL) [11,12]. When an object with a linear photo-response is imaged, the resolution of these techniques is fundamentally limited to approximately $\lambda_0/4$ [13]. The imaging of unknown objects with deep sub-wavelength resolution is still

predominately performed by relatively slow near-field scanning optical microscopy (NSOM) [14].

There exist several theoretical proposals to achieve fast imaging with sub-wavelength resolution in diffractive and tomographic set-ups [15,16]. In grating-assisted ODT [17] and interscale mixing microscopy (IMM) [18,19] a diffractive element is employed to out-couple information about sub-wavelength features of an object into the far field — similarly to SIM — with the final image formed with the post-processing of information carried by multiple diffractive orders (Fig.1b) by analyzing either full electromagnetic field (ODT [17]) or intensity (IMM [18,19]). Although IMM somewhat resembles SIM and FSL, in contrast to the latter approaches, IMM utilizes multiple diffractive orders of the grating and therefore provides a resolution that is limited only by experimental noise. Here we report an experimental realization of the IMM with both coherent ($\lambda_0 = 532 \text{ nm}$) and incoherent ($600 \leq \lambda_0 \leq 800 \text{ nm}$) illumination, achieving a resolution of the order of 70 nm ($\sim \lambda_0/10$) with far-field measurements which do not require point-by-point imaging. Moreover, we present a simple analytic technique to post-process the resulting information, often on the basis of a *single* diffractive measurement. The formalism presented here opens the avenue for far-field microscopy and spectroscopy of nanoscale objects.

Mathematically, the process of imaging is equivalent to recovering the distribution of electromagnetic waves at the location of the object.

For one-dimensional objects, this distribution can be described by a plane-wave spectrum parameterized by the transverse component of wavevector k_x with wavevector-dependent amplitude $\vec{E}(k_x)$ (2D objects and combinations of small 3D objects can be considered similarly [19])

$$\vec{E}(\vec{r}) = \int_{-\infty}^{\infty} \vec{E}(k_x) e^{i\vec{k}\cdot\vec{r} - i\omega t} dk_x \quad (1)$$

where ω is angular frequency, and \vec{k} is the wavevector of the component of the wave. Since the components of the wavevector in free space are related to each other via $k_x^2 + k_z^2 = 4\pi^2/\lambda_0^2$, and since information on the length-scale L is encoded into wavevectors with $k_x \sim 2\pi/L$, (Figure 1) the information about the sub-wavelength features of the object is encoded in the evanescent, non-propagating waves which exponentially decay away from the source. As the distance to the object increases, the “signal” about the subwavelength features gets exponentially suppressed by the diffraction-limited “background” and experimental noise. Therefore, the resolution of far-field optical microscopy is directly related to the signal-to-noise ratio of the measurements.[20] Sparsity-based imaging [21] fills-in the sub-wavelength information based on an analytic continuation of available diffraction-limited measurements of relatively sparse (isolated) objects.

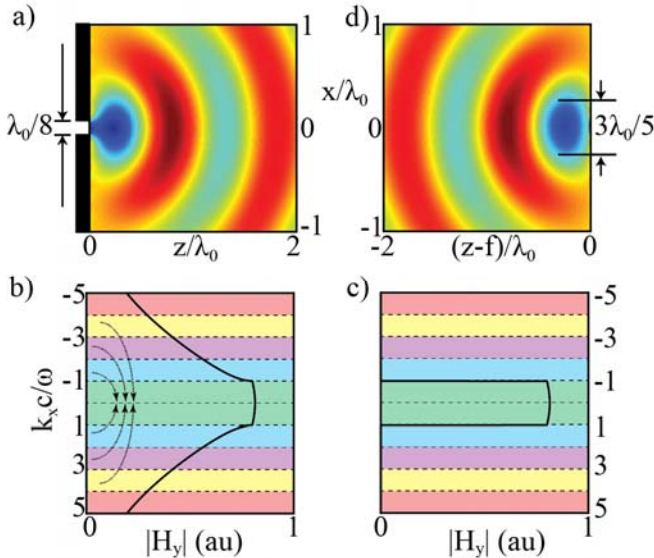


Figure 1: Light scattered by an object (slit in this example) can be represented as a collection of plane waves parameterized by the transverse wavevector k_x ; The Fourier spectrum of a sub-wavelength object is dominated by evanescent modes with $\frac{k_x c}{\omega} > 1$ (a,b). As the light propagates to the far-field of the object, the evanescent components get exponentially suppressed (c). Attempts to optically reconstruct the image in the far-field result in a diffraction-limited pattern (d). IMM mixes evanescent information into the propagating part of the spectrum [arrows in (b)], enabling to distinguish information about sub-wavelength features of the source with far-field measurements.

For densely placed objects, several techniques aim at enhancing the signal carried by evanescent-waves. NSOM collects the near-field information directly, at a cost of slow, point-by-point imaging. The concept of superoscillations [22,23], band-limited functions which oscillate faster than its fastest Fourier component have also been instrumental in achieving sub-wavelength resolution in the scanning microscopy regime. Superlenses [11], hyperlenses[24,25,26], and other metamaterial-based direct imaging solutions have been used to propagate evanescent information in a relatively narrow frequency ranges where (a component of) the permittivity of the metamaterial is close to its plasmon resonance (superlens) or zero (hyperlens). In

addition, the metamaterial solutions that provide magnification typically have rather limited field of view.

Alternatively, information about $k_x \gg 2\pi/\lambda_0$ can be diffracted into the propagating waves and thus be directly measured in the far field with no need to perform point-by-point scanning. The use of periodic structures to achieve super-resolution was first investigated a half-century ago by using multiple gratings in order to generate a structured light beam and then using the diffraction of this beam by the object to gain access to the evanescent part of the spectrum. [27,28] Today, diffraction-based characterization allows the analysis of the profile of highly periodic diffracting structures with a resolution of the order of single nm. [29,30] Structured illumination microscopy [8,31] allows the imaging of unknown objects with $\lambda_0/4$ resolution at the expense of multiple measurements and computer post-processing. The far-field superlens [32] uses near field excitation of an object along with resonantly enhanced fields of surface plasmons to achieve $\sim \lambda_0/5$ resolution. Since both SIM and FSL utilize only first order diffraction (for non-fluorescent samples; higher order SIM is only possible on fluorescent samples [33]), these resolution limits cannot be further improved within the existing frameworks.

Optical Diffraction Tomography, a technique that aims to analyze the internal structure of transparent objects based on multiple measurements of the light scattered by the object is becoming powerful for analysis of some biological samples [10]. However, stable and reasonably fast reconstruction of ODT measurements is fundamentally similar to resolution of SIM and is applicable primarily to analysis of low-scattering (low index contrast) samples.

Several extensions of ODT to two-dimensional tomography with subwavelength resolution recently proposed theoretically [15,17]. However, the majority of these techniques requires measurements of both field amplitude and phase in order to reconstruct the image, which is accomplished by fitting measured data to simulations [17]. While possible in theory, such fittings are typically prone to both numerical and experimental noise, especially since optical phase can rarely be measured directly.[15,34] It is likely that practical realization of such techniques will require prohibitively extensive characterization of both the sample, the scattering environment, as well as response function of the particular optical setup[29]. Even then, recovery of optical phase may be a great challenge.

Interscale mixing microscopy (IMM), first proposed in Ref. [18] relies on a diffraction element — positioned in the near field proximity to an object — to fold the evanescent information into the propagation zone (Figure 1). Such folding essentially mixes the information about sub-wavelength features of the object with the information about diffraction-limited features. Since, in contrast to SIM and FSL, IMM uses multiple diffraction orders, it can in principle achieve unlimited resolution. In practice, the resolution of IMM is limited by the ability to resolve high-order diffracted signal among the zero-order diffracted background. It has been shown, numerically, that realistic diffracting structures enable up to $\lambda_0/20$ resolution that is limited by experimental noise and instabilities in numerical calculations that can be somewhat mitigated with multiple measurements.[19]

Several algorithms for recovering the information about the object based on post-processing of the multiple measurements of field [17] or intensity [18,19] profile have been developed. It was shown that when the scattering by an unperturbed diffraction grating is characterized well enough to be reproduced numerically, image recovery can then be mapped to an optimization problem that minimizes the deviation between the predicted optical response of the test object in front of the unperturbed diffraction element and the measured signal. However, as suggested by previous experimental studies [29], such characterization provides extreme constraints on experimental setup. Analysis of our experimental data is consistent with these assessments.

In this work, the problem of image recovery in IMM is addressed by the development of new, straightforward analytic signal-processing technique which allows pinpointing of the diffractive signatures of the object and isolate these signatures from the (relatively strong)

background created by the diffraction element. As result, we show that only a *single measurement* may be sufficient to achieve, theoretically and experimentally, deep sub-wavelength resolution with IMM.

2. Experimental Setup

A series of finite gratings (25 periods) were fabricated on a thin (100 nm) gold film on a glass substrate. Two different sets of samples, with periods $\Lambda = 325 \text{ nm}$ and $\Lambda = 275 \text{ nm}$, each having a slit width of 125 nm were fabricated. Each set contains three structures: (i) a reference, perfectly periodic grating, (ii) a grating with an absent slit in the center, and (iii) a grating with a slit misplaced by $\sim \Lambda/4$ (Fig. 2). Apart from the scaling, the results from samples of two different periods are similar to each other. Here we present results for the set of samples with smaller period, where the smallest defect was on the order of $\sim 70 \text{ nm}$. The samples were characterized using a 532 nm CW laser, as well as with a broad-band incoherent white-light illumination 600–800 nm, putting the smallest size of the defect in the range of $\lambda_0/7$ – $\lambda_0/10$. For the measurements, the samples were illuminated with a 40x objective (0.95 NA) using a quasi-plane wave obtained by focusing the light at the back focal plane of the objective (Fig. 2). The incidence angle was controlled by a pair of galvanometric mirrors conjugated to the focal plane of the illumination objective and the scattered light was detected in transmission using a 100x objective (1.49 NA). The back focal plane of the detection objective (which corresponds to the Fourier plane) was then directly imaged onto an imaging spectrometer. Coherent measurements were performed by imaging the back focal plane directly onto the camera, while white-light measurements were performed with a 300 μm wide slit used to select only the specular transmission in the axis perpendicular to the grating, producing far-field diffraction pattern as a function of wavelength.

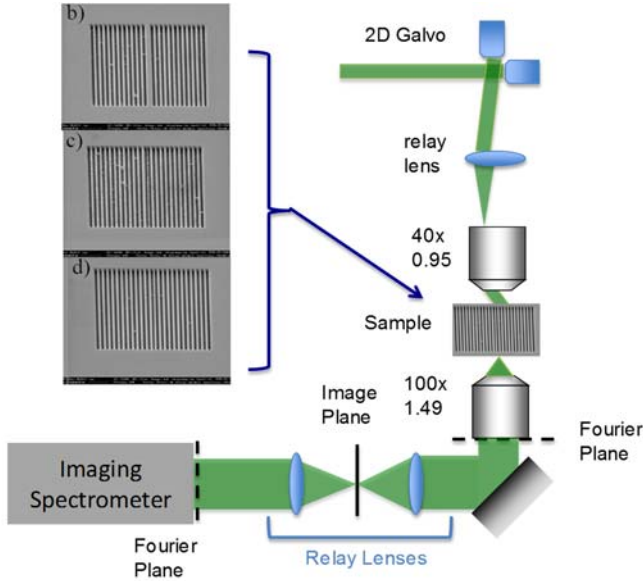


Figure 2: (a) Experimental optical imaging setup; (b)-(d) fabricated gratings with $\Lambda = 275 \text{ nm}$: (b) centered defect; (c) off-center defect; (d) no defects

3. Theoretical analysis

Numerical extraction of information about the unknown object was suggested as a basis for IMM in previous studies [18,19]. However, it was shown that in practice the implementation of such algorithms require extreme efforts in equipment calibration [19,30]. Here we present a new, analytic implementation of IMM. The reference diffraction element used in this work represents a finite grating with $N = 25$ slits with width w and period Λ . The field generated in the

near-field proximity of such a grating, illuminated by a single, normally incident plane wave, is given by

$$H_y(x) = \sum_{n=-\frac{N-1}{2}}^{\frac{N-1}{2}} \text{rect}\left(\frac{x}{w}\right) * \delta(x - n\Lambda) \quad (2)$$

with $*$ denoting the convolution operation, $\text{rect}(\xi)$ being the rectangular step function, and $\delta(\xi)$ being the Dirac delta function. The (magnetic) field in the far-field regime is well-approximated by Fraunhofer scalar diffraction theory and is best characterized in the Fourier domain as

$$H_y(k_x) = w \text{sinc}\left(\frac{k_x w}{2}\right) \frac{\sin\left(\frac{N k_x \Lambda}{2}\right)}{\sin\left(\frac{k_x \Lambda}{2}\right)} \quad (3)$$

When an object (e.g., grating defect) of size l is added to the grating, it modifies the field generated by the grating by adding (or subtracting) the field of the object, $H_y^d(x) = \text{rect}\left(\frac{x}{l}\right) * \delta(x - a)$. As result, the far-field is modified as well:

$$H_y(k) = w \text{sinc}\left(\frac{k w}{2}\right) \frac{\sin\left(\frac{N k \Lambda}{2}\right)}{\sin\left(\frac{k \Lambda}{2}\right)} + l \text{sinc}\left(\frac{k l}{2}\right) e^{-i k a} \quad (4)$$

The vast majority of optical measurements rely on detecting the intensity, not the field itself. The total intensity measured by the detector is proportional to

$$I(k_x) \propto |H_y(k_x)|^2 = \frac{I_g(k_x) + I_d(k_x) + I_i(k_x)}{\sin^2\left(\frac{k_x \Lambda}{2}\right)} \quad (5)$$

where

$$\begin{aligned} I_g(k_x) &= w^2 \text{sinc}^2\left(\frac{k_x w}{2}\right) \sin^2\left(\frac{N k_x \Lambda}{2}\right) \\ I_d(k_x) &= l^2 \text{sinc}^2\left(\frac{k_x l}{2}\right) \sin^2\left(\frac{k_x \Lambda}{2}\right) \\ I_i(k_x) &= 2 w l \text{sinc}\left(\frac{k_x w}{2}\right) \text{sinc}\left(\frac{k_x l}{2}\right) \sin\left(\frac{k_x \Lambda}{2}\right) \\ &\quad \times \sin\left(\frac{N k_x \Lambda}{2}\right) \cos(k_x a) \end{aligned} \quad (6)$$

The first of these terms represents the spectrum of an ideal grating and dominates the far-field intensity, especially in the proximity of diffraction maxima ($k\Lambda \approx 2\pi n$). The second term describes the (relatively weak) contribution of the object in the absence of the grating. The last term corresponds to the interference between the fields of the ideal grating and the object. The physics behind the IMM can now be clearly seen from analysis of relative amplitudes of the three terms: while the direct scattered contribution to the signal from the object is small, the grating-object interaction enhances the far field contribution from the object by a factor of $w/l \gg 1$.

The equations above can be used to illustrate the difference between the IMM and SIM-like diffraction techniques. In the IMM formalism, the sample is interrogated by a single plane wave, and signal processing is focused on the cancellation of all principal diffracted beams, analyzing the interference in the ringing tails of the principle orders. As a result, the information about the object can be extracted based on single measurement. In contrast, in SIM-like techniques the sample is interrogated by multiple beams, and the measurement aims at detecting the zero-order interference, which needs to be post-processed and requires multiple measurements.

On the implementation level, the signal-carrying interference term can be enhanced by analyzing the product $I(k_x) \sin^2(k_x \Lambda/2)$ that suppresses the intensity around the diffraction maxima of the ideal grating. The spatial profile and the position of the object can be analyzed by considering the Fourier transform of the power spectrum

$$I(x) = \left| F \left[I(k_x) \sin^2 \left(\frac{k_x \Lambda}{2} \right) \right] \right|^2 \quad (7)$$

which formally translates the spectrum from wavevector- into real-space domain.

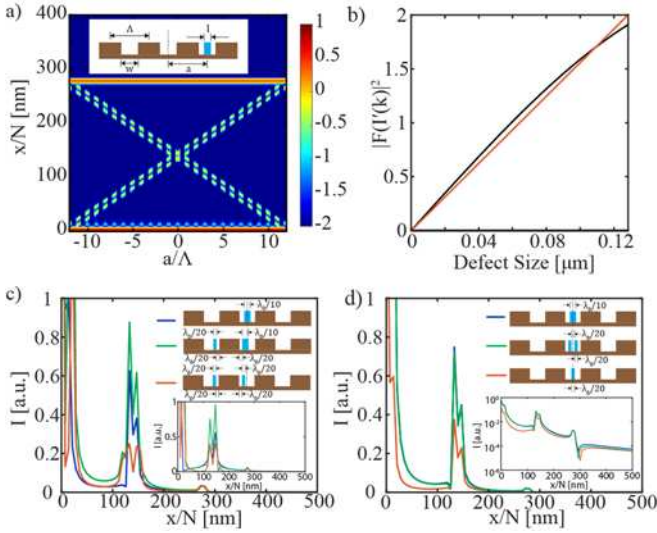


Figure 3: IMM signal [Eq.(7)] for a point object that is being moved from one end to another end of the finite diffraction grating [inset in (a)]: (a) the dependence of the IMM signal on defect position for object size $\lambda_0 = 532\text{nm}$, $l = \lambda_0/20$ in $\Lambda = 275\text{nm}$; $N = 25$ grating; (b) the dependence of the IMM maximum at $a/\Lambda = 0$ on object size l (black line); red line in (b) shows linear dependence; (c) IMM signal for the setup in (a) for defects in neighboring apertures [inset shows the IMM signal of the same sample interrogated with $\lambda_0 = 800\text{nm}$ light] (d) IMM signal for the setup in (a) for objects within the same aperture. [inset shows the signal in logarithmic scale]

The use of the Fourier transform to post-process optical measurements is a common practice in ODT, SIM, and now IMM. However, we note again that the implementation of IMM proposed here is distinct from both ODT and SIM. Thus, ODT explicitly relies on small index contrast between the sample and the environment. SIM and IMM do not have this limitation. At the same time, IMM provides significant resolution enhancement as compared to both SIM, and ODT.

Fig.3 illustrates the performance of IMM, as defined by Eq.(7) for several representative objects. The operating wavelength, geometry of the grating, and data sampling rate reflect those used in our experimental setup. First, we consider the evolution of the Fourier spectrum of a grating with a single object as the object is moved across the grating. For a fixed position of the object (inset in Fig. 3a), the signal $I(x)$ has two main features. The first is a maximum located at $N\Lambda$ that corresponds to the period of the grating and represents the contribution from the main diffraction peak. The second feature represents the interaction of the object with the grating. Its position is directly related to the position of the object with a resolution of the order of the slit of the grating. Its intensity, in the limit $l \ll w$, is proportional to the size of the defect (Figure 3b). When the object size approaches the size of the grating slit, the intensity dependence on the size slowly deviates from a linear relationship. The signal from the object itself, ($\propto l^2$ term in Eq.(6)) is not seen in these spectra.

Note that (i) the signatures of sub-wavelength objects can be clearly resolved and (ii) the Fourier spectrum, constructed according to Eqs.(5...7), represents a direct measurement of both position and size of the object with sub-wavelength accuracy.

The product $I(k_x) \sin^2 \left(\frac{k_x \Lambda}{2} \right)$ [see Eqs. (5,6)] determines the true resolution of the imaging system. The first term representing the ideal grating will have its centroid located at double the frequency of the interference term due to the square of the dominant sine term. The secondary peak is related to the position of the object, with a symmetry about $x = \frac{N\Lambda}{2}$. Taken together, the positions of these maxima allow a precise calibration of the diffraction element and a measurement of the position of the object with relationship to the diffracting element with a great accuracy. Separate calibration (for example, using diffraction grating with one missing slit), can be used to determine the sizes of the unknown objects as well as their positions.

The aforementioned symmetry about $x = N\Lambda/2$ yields ambiguity of the sign of the object displacement from the center of the diffractive element and thus represents a limitation of the current implementation of IMM. This ambiguity can be avoided in a non-static arrangement where the imaging target, as moving the object over the periodic aperture, would break the $\pm x$ symmetry and provides unambiguous position measurement of the object. Alternatively, the ambiguity can be avoided by restricting the operational field of view of IMM systems.

The proposed recovery procedure allows for imaging of composite objects. Thus, Fig.(3c) clearly shows that Eq.(7) can be used to differentiate between an isolated $\lambda_0/10$ object and two objects, $\lambda_0/10$ and $\lambda_0/20$, positioned in the neighboring openings of the grating. The total scattered signal represents the combined size of the objects, while the spatial distribution of the secondary diffracted peaks reflects the locations of the parts of the composite object. Therefore, with proper calibration, it is possible to determine both the size and the locations of these objects (with exception of the position ambiguity mentioned above). One of the main conclusions of the proposed theoretical analysis is that reducing the period of the grating represents a straightforward way to improve resolution of IMM formalism.

Fig.(3d) compares the diffractive signal of isolated $\lambda_0/10$ and $\lambda_0/20$ objects and two $\lambda_0/20$ objects within the same opening of the diffraction grating. It is seen that with further signal processing it may be possible to recover the composite objects located within the same opening. We defer the development of such signal processing and its experimental validation to our future work.

4. Results

The diffraction patterns for the structures under consideration were experimentally measured and simulated using Eq. (7). Two different types of measurements were analyzed.

In the first set of measurements, the samples were interrogated with coherent $\lambda = 532\text{nm}$ light, for different incident angles. To compare the predictions of theoretical analysis to experimental spectra, experimental data from CCD images was translated to superimpose the data corresponding to different incident angles. The resultant k_x spectra were Fourier-transformed to convert the angular information into the real-space domain according to Eq. (7). Fig. 4a illustrates the result of post-processing a single measurement. Fig. 4b represents the statistics of 9 measurements corresponding to different incident angles. Fig. 4c shows theoretical predictions according to Eq. (7). It is seen that experimental data are in good agreement with theoretical predictions, with positions of the diffracted peaks representing positions of the objects in the middle of the grating, and the ratio of the amplitudes representing the ratio of the dimensions of the defects Sample 1 [$\sim 130\text{nm}$] and Sample 2 [$\sim 70\text{nm}$], respectively. It is clearly seen that IMM can resolve $\sim 70\text{-nm}$ -scale defects. Interestingly, a single measurement provides enough information to resolve the defect.

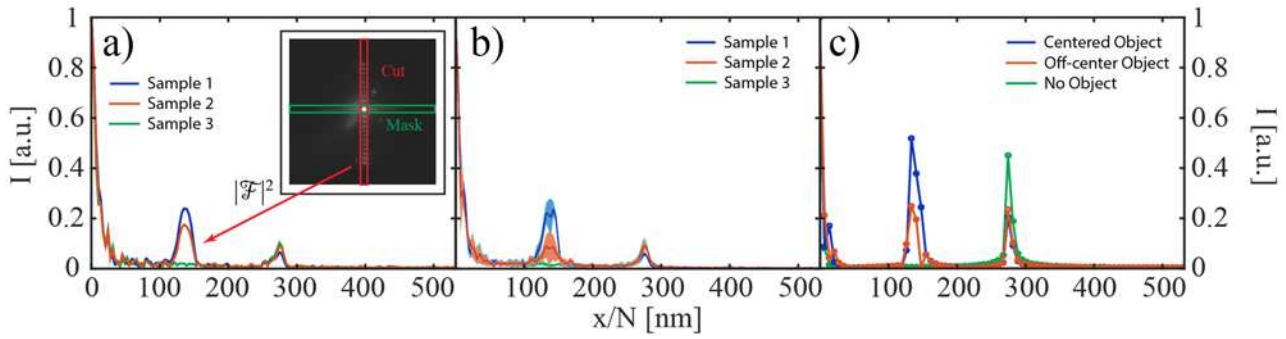


Figure 4: IMM signal based on (a) single experimental measurement corresponding to an incident angle of 21° , (b) post-processed experimental data of 9 different incident angles, and (c) theoretical predictions of $|\mathcal{F}[I'(k)]|^2$ according to Eq.(7). The position of diffracted peaks and the ratio of their amplitudes represent position and relative dimensions of the objects. Thick lines and shaded areas in (b) represent the mean and standard deviation of post-processed data respectively; in all panels $\Lambda = 275\text{nm}$, $\lambda_0 = 532\text{nm}$. Inset in (a) illustrates the typical imaging processing routine: starting from the raw CCD image, we extract the transmission perpendicular to the grating, suppress the main diffraction peaks by multiplying the signal by $\sin(k\Lambda/2)^2$, followed by Fourier transformation of the power spectrum.

In the second set of measurements, the sample was illuminated by a broadband incoherent source. Prior to translation, the contrast of raw CCD images was enhanced by subtracting the background and the images were de-skewed to compensate for misalignment of the optical setup (this eliminated a small, $\sim 5/250$ drift of the image). The resulting experimental data is compared to theoretical predictions in Fig. 5. Once again, it is seen that the predictions of Eq. (7) are in agreement with experimental data and that both half-period and quarter period defects can be clearly distinguished from the ideal grating and from each other. The spectrum of the defect-free grating has a single wavelength-independent peak representing the period of the grating. The spectra of the two samples with defects contain additional features. The location of these features represent the position of the defect (central slit of the grating), while their structure describes the characteristic of the defect: the missing slit sample yields a double-peak pattern, the shifted slit yields a more complex, broader (but lower amplitude) spectrum maximum. Note that due to the mutual alignment of optical elements and CCDs the broadband spectra provide approximately 4 times the number of k_x datapoints for each wavelength as compared to single-wavelength setup. As result, the fine-structure of the IMM signal can be resolved much better in Fig.5 than in Fig.4.

5. Discussion and conclusions

We have demonstrated that by using multiple diffractive orders of a grating in the near-field proximity to a nanoscale object, it is possible to recover deep sub-wavelength information, usually lost in the evanescent wave spectrum, with the far-field measurements. A simple analytic technique capable of predicting the position and size of the opaque object in close proximity to a diffractive element has been developed and validated in the experiments. The resolution is related to recovering the parameters of the full spatial spectrum of light diffracted by the sample and grating system. Resolution of the order of $\sim \lambda_0/10$ has been achieved experimentally. Notably, the developed formalism has been shown to work for both coherent and incoherent excitation, opening the pathway to the spectroscopy of nanoscale objects.

In practical imaging systems, the period of the grating and its duty cycle need to be optimized as smaller period generally yields better resolution while at the same time potentially decreases signal-to-noise ratio.

The approach presented here for one-dimensional objects can be extended to the imaging and spectroscopy of two-dimensional

structures with the help of 2D diffractive elements. In order to achieve reliable recovery of two-dimensional objects, future studies will need to identify the stability of such recoveries with respect to the shape of the diffractive element (circular vs rectangular vs hexagonal gratings), the Fourier/Bessel transform used, as well as the robustness of the signal recovery with respect to noise and imperfections of optical setup. These studies, although not trivial, are fundamentally similar to the approach used in this work.

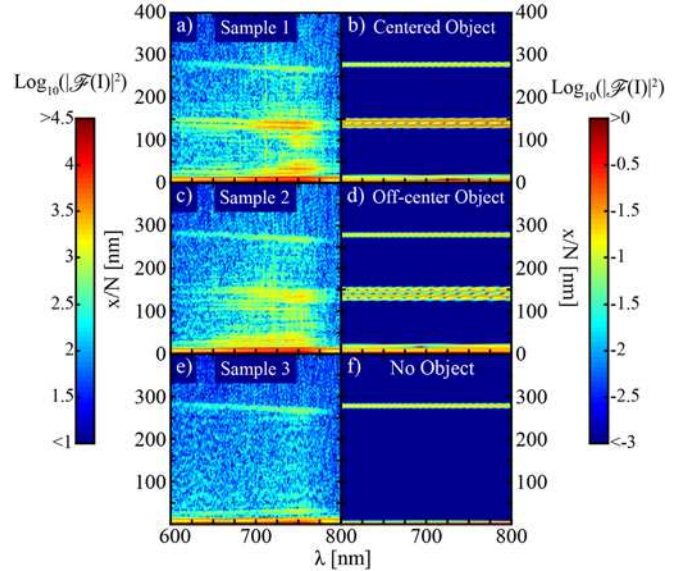


Figure 5: IMM signal extracted from broadband experimental data (a,c,e) and calculated using Eq.(7) (b,d,f) for samples with missing slit (a,b), shifted slit (c,d), and defect-free grating (e,f).

Finally, we note that in realistic objects, the presented formalism will measure the combination of the geometrical size and optical transparency of the object. The spectral dependence of this product, determined by the developed formalism, provides the direct measurement of the spectral response of the nanoscale object.

Funding This research was sponsored, in part, by NSF (grants ## ECCS-1102183 and DMR-1209761) and EPSRC (U.K.). A.Z. acknowledges support from the Royal Society and the Wolfson Foundation. The data access statement: all data supporting this research are provided in full in the results section.

1. E. E. Abbe, "Beiträge zur Theorie des Mikroskops und der mikroskopischen Wahrnehmung," *Archiv für Mikroskopische Anatomie*, **9**, 413-418, (1873).

2. L. Rayleigh, "On the theory of optical images, with special reference to the microscope," *Philosophical Magazine*, **42**, 167-195, (1896).

-
3. M. Born and E. Wolf, *Principles of Optics: Electromagnetic Theory of Propagation, Interference, and Diffraction of Light*, (Cambridge University, 1999).
 4. M.J. Rust, M Bates, and X Zhuang. "Sub-diffraction-limit imaging by stochastic optical reconstruction microscopy (STORM)." *Nature methods* **3.10** 793-796, 2006
 5. E. Betzig, et al. "Imaging intracellular fluorescent proteins at nanometer resolution." *Science* **313**, 5793, 1642-1645, (2006)
 6. S.T. Hess, T.P.K. Girirajan, and M.D. Mason. "Ultra-high resolution imaging by fluorescence photoactivation localization microscopy." *Biophysical journal* **91**, 11, 4258-4272, (2006).
 7. S.W. Hell, and J. Wichmann. "Breaking the diffraction resolution limit by stimulated emission: stimulated-emission-depletion fluorescence microscopy." *Optics letters* **19**, 11, 780-782 (1994).
 8. M.G.L. Gustafsson, "Surpassing the lateral resolution limit by a factor of two using structured illumination microscopy." *Journal of microscopy* **198**, 2 82-87, (2000).
 9. A.C. Kak, M. Slaney, *Principles of Computerized Tomographic imaging*, (Acad press, New York, 1999)
 10. T. Kim, R. Zhou, M. Mir, S.D. Babacan, P.S. Carney, L.L. Goddard, and G. Popescu. "White-light diffraction tomography of unlabelled live cells." *Nature Photonics* **8**, 256-263, (2014).
 11. S. Durant, Z. Liu, J. Steele, and X. Zhang, "Theory of the transmission properties of an optical far-field superlens for imaging beyond the diffraction limit," *J. Opt. Soc. Am. B* **23**, 2383-2392, (2006).
 12. Z. Liu, S. Durant, H. Lee, Y. Pikus, N. Fang, Y. Xiong, C. Sun and X. Zhang, "Far-field optical superlens," *Nano Letters*, **7**, 2, 403-408, (2007).
 13. A.S. Kewitsch, and A Yariv, "Nonlinear optical properties of photoresists for projection lithography," *Applied Physics Letters*, **68**, 455-457 (1996)
 14. U.Durig, D. W. Pohl and F. Rohner, "Nearfield optical scanning microscopy," *Journal of Applied Physics*, **59**, 3318-3327, (1986).
 15. P. S. Carney, V. A. Markel and J. C. Schotland, "Near-field tomography without phase retrieval," *Physical Review Letters*, **86**, 5874-5877, (2001).
 16. A. A. Govyadinov, G. Y. Panasyuk and J. C. Schotland, "Phaseless three-dimensional optical nanoimaging," *Physical Review Letters*, **103**, 213901, (2009).
 17. A. Sentenac, P. Chaumet and K. Belkebir, "Beyond the Rayleigh Criterion: Grating Assisted Far-Field Optical Diffraction Tomography," *Physical Review Letters*, **97**, 24, (2006).
 18. S. Thongrattanasiri, N. A. Kuhta, M. D. Escarra, A. J. Hoffman, C. F. Gmachl and V. A. Podolskiy, "Analytical technique for subwavelength far field imaging," *Applied Physics Letters*, **97**, 10, (2010).
 19. S. Inampudi, N. Kuhta and V. A. Podolskiy, "Interscale mixing microscopy: numerically stable imaging of wavelength-scale objects with sub-wavelength resolution and far field measurements," *Optics express*, **23**, 3, 2753-2763, (2015).
 20. E. E. Narimanov, "The resolution limit for far-field optical imaging," in *2013 CLEO Technical Digest*, (Optical Society of America, 2013), paper QW3A.7.
 21. A. Szameit, Y. Shechtman, E. Osherovich, E. Bullkich, P. Sidorenko, H. Dana, S. Stiener, E. B. Kley, S. Gazit, T. Cohen-Hyams, S. Shoham, M Zibulevsky, I. Yavneh, Y. C. Eldar, O. Cohen and M. Segev, "Sparsity-based single-shot subwavelength coherent diffractive imaging," *Nature materials*, **11**, 5, 455-459, (2012).
 22. E. T. F. Rogers, J. Lindberg, T. Roy, S. Savo, J. Chad, M. Dennis and N. I. Zheludev, "A super-oscillatory lens optical microscope for subwavelength imaging," *Nature materials*, **11**, 5, 432-436, (2012).
 23. M. V. Berry and S. Popescu, "Evolution of quantum superoscillations and optical superresolution without evanescent waves," *Journal of Physics A: Mathematical and General*, **39**, 22, 6965, (2006).
 24. Z. Jacob, L. Alekseyev, and E. Narimanov, "Optical Hyperlens: Far-field imaging beyond the diffraction limit," *Optics Express*, **14**, 8247-8256 (2006).
 25. A. Salandrino and N. Engheta, Far-field subdiffraction optical microscopy using metamaterial crystals: theory and simulations, *Phys. Rev. B*, **74**, 075103, (2006).
 26. Z. Liu, H. Lee, Y. Xiong, C. Sun, and X. Zhang, Far-field optical hyperlens magnifying sub-diffraction-limited objects, *Science*, **315**, 1686, (2007).
 27. M. A. Grimm and A. W. Lohmann, "Superresolution Image for One-Dimensional Objects," *Journal of the Optical Society of America*, **56**, 9, (1966).
 28. W. Lukosz, "Optical Systems with Resolving Powers Exceeding the Classical Limit," *Journal of the Optical Society of America*, **56**, 11, (1966).
 29. R. M. Silver, B. M. Barnes, A. Ravikiran, J. Jun, M. Stocker, E. Marx and H. J. Patrick. "Scatterfield microscopy for extending the limits of image-based optical metrology." *Applied optics*, **46**, 20 4248-4257, (2007).
 30. J. Qin, R. M. Silver, B. M. Barnes, H. Zhou and F. Goasmat, "Fourier domain optical tool normalization for quantitative parametric image reconstruction," *Applied Optics*, **52**, 26, 6512-6522, (2013).
 31. E. Sabo, Z. Zalevsky, M. David, N. Konforti and I. Kiryuschev, "Superresolution optical system using three fixed generalized gratings: experimental results," *Journal of the Optical Society of America A*, **18**, 3, (2001).
 32. Z. Liu, S. Durant, H. Lee, Y. Pikus, N. Fang, Y. Xiong, C. Sun and X. Zhang, "Far-field optical superlens," *Nano Letters*, **7**, 2, 403-408, (2007).
 33. M.G.L. Gustafsson, "Nonlinear structured-illumination microscopy: wide-field fluorescence imaging with theoretically unlimited resolution." *Proceedings of the National Academy of Sciences of the United States of America* **102**, 37, 13081-13086, (2005).
 34. W. M. J. Coene, A. Thust, M. O. De Beeck and D. Van Dyck, "Maximum-likelihood method for focus-variation image reconstruction in high resolution transmission electron microscopy," *Ultramicroscopy*, **64**, 1, 109-135, (1996).