

This is a repository copy of *Plasma temperature measurements using black-body radiation from spectral lines emitted by a capillary discharge*.

White Rose Research Online URL for this paper:

<https://eprints.whiterose.ac.uk/id/eprint/135534/>

Version: Accepted Version

Article:

Tallents, Gregory John orcid.org/0000-0002-1409-105X, Wilson, Sarah Arabella orcid.org/0000-0001-5914-5085, Wagenaars, Erik orcid.org/0000-0002-5493-3434 et al. (2 more authors) (2018) Plasma temperature measurements using black-body radiation from spectral lines emitted by a capillary discharge. *Journal of Quantitative Spectroscopy and Radiative Transfer*. ISSN: 0022-4073

<https://doi.org/10.1016/j.jqsrt.2018.09.005>

Reuse

This article is distributed under the terms of the Creative Commons Attribution-NonCommercial-NoDerivs (CC BY-NC-ND) licence. This licence only allows you to download this work and share it with others as long as you credit the authors, but you can't change the article in any way or use it commercially. More information and the full terms of the licence here: <https://creativecommons.org/licenses/>

Takedown

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing eprints@whiterose.ac.uk including the URL of the record and the reason for the withdrawal request.

Plasma temperature measurements using black-body radiation from spectral lines emitted by a capillary discharge

T. Page, S. A. Wilson, J. Branson, E. Wagenaars and G. J. Tallents

York Plasma Institute, Department of Physics, University of York, York YO10 5DD, U.K.

Abstract

Optically thick spectral line emission from plasmas is often difficult to use for the diagnosis of plasma parameters. We demonstrate a technique for temperature measurement using the peak intensity of optically thick lines as their intensities approach a black-body distribution. Recording optical emission in the wavelength range 300 - 1000 nm from a plasma formed by radio-frequency heating and electrical discharges in a 0.2 m long capillary plasma, we show that the high wavelength Rayleigh-Jeans form of the black-body emission can be fitted to the most intense spectral lines to give a measurement of plasma temperatures in the 1 - 1.5 eV range. The temperature measurement technique should have wider applicability in diagnosing plasmas with optically thick spectral lines.

Keywords: opacity, Rayleigh-Jeans, black-body, plasma

1. Introduction

Capillary discharge plasmas have several potential and realised applications. The plasmas produced in a capillary discharge are very uniform along the capillary length, enabling, for example, basic studies of atomic kinetics and radiation transfer without the complications of non-uniformity as occurs in, for example, many laser-produced plasmas [1]. Capillary discharge plasmas have been proposed as appropriate plasmas for the propagation and guiding of injected laser pulses with the aim of generating wake-fields suitable for the acceleration of

electrons with acceleration gradients $> 100 \text{ GeV m}^{-1}$ [2], [3], [4]. Plasma escap-
10 ing along the axis of the capillary has been proposed for medical applications,
including sterilization [5]. With tailored high current discharges, plasmas with
peak electron temperatures of 350 eV have been produced in capillary discharge
plasmas [6].

Lasing at wavelength 46.9 nm in the extreme ultra-violet has been achieved
15 using capillary discharge plasmas [7], [8], with several applications of the laser
output now being developed (for example, see [9], [10]). Amplified spontaneous
emission occurs along typically 0.2 m of argon plasma ionised and excited by
sequences of radio-frequency heating and electrical discharges. The physics of
a capillary discharge plasma is similar to more conventional Z-pinch designs,
20 but with a solid capillary acting as a physical guide for the electrical current
[11]. Electron temperatures in the pinch plasma can approach 80 eV for times
of several nanoseconds and enable the production of population inversions in
Ne-like argon leading to lasing at 46.9 nm [7], [8]. However, the spatially and
temporally averaged emission from the argon plasma in the visible/near infra-
25 red spectral range is dominated by a much longer lived, much lower temperature
plasma not associated with the plasma pinching effect.

In this paper, we measure the electron temperatures associated with the
unpinched plasma for a capillary discharge. The visible/near infra-red emission
from the capillary arises from plasma formed without significant pinching, while
30 the pinched plasma temperature (up to 80 eV) produces emission from ions such
as Ne-like argon in the extreme ultra-violet and soft x-ray spectral regions.

2. Background: emission from uniform optically thick plasmas

For the capillary discharge used for the present study, plasma is formed by
a radio-frequency discharge in argon gas of pressure 0.3 Torr contained in the
35 bore of a ceramic capillary of inner diameter 3 mm. Singly ionised argon (Ar
II) is created with emission of neutral and singly ionised argon occurring for
durations up to a millisecond. For a much shorter duration of several nanosec-

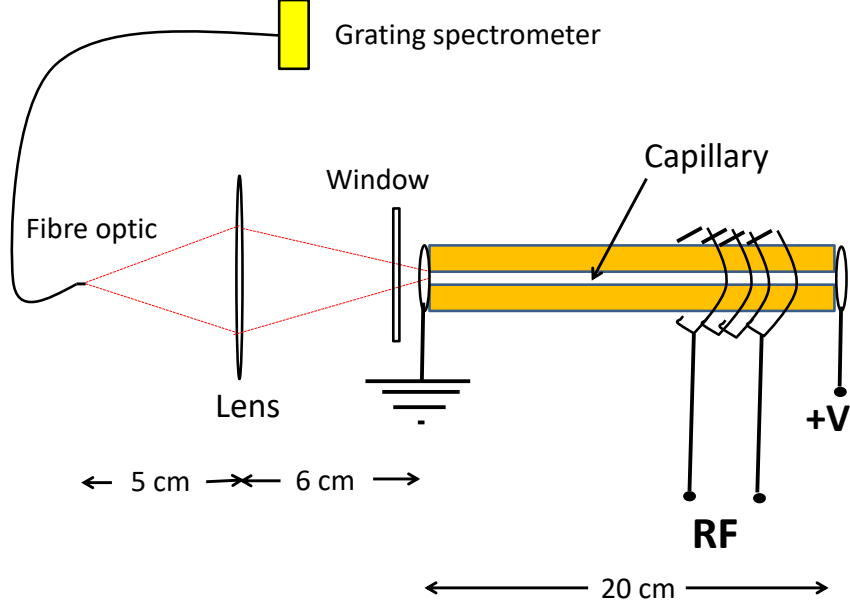


Figure 1: A schematic of the argon filled (0.3 Torr) capillary with radio-frequency (RF) heating coil and electrodes for high voltage direct current discharge down the 3 mm diameter bore of the capillary. Optical spectra are recorded by focusing the plasma emission onto an optical fibre connected to a 300 lines/mm grating spectrometer with CCD detection. Vacuum and electrical pulse forming components are not shown. The glass window separates the argon gas and atmospheric air.

onds, a current flow of up to 40 kAmps creates a plasma pinch with electron densities $\approx 10^{19} \text{ cm}^{-3}$ and diameter $\approx 100 \mu\text{m}$. The capillary discharge plasma
40 is approximately uniform along the capillary axis for a distance of $\approx 0.2 \text{ m}$ (see figure 1).

For a plasma with a constant source function S_0 along a line of sight, the intensity I of radiation escaping the plasma is given by

$$I = S_0(1 - \exp(-\tau)) \quad (1)$$

where τ is the optical depth along the line of sight. Kirchhoff's law states that
45 the source function S_0 is equal to the Planck black-body radiation intensity I_p

with the radiation temperature equal to the electron temperature [12]. Consequently following equation 1, the maximum value of the intensity I at any wavelength approaches the black-body intensity I_p as the optical depth τ increases. On a line of sight along the axis of a capillary discharge plasma, the
50 optical depth at the line centre of optical spectral line emission is high, whereas the optical depth of continuum emission between the spectral lines is close to optically thin. The most optically thick spectral components of plasma intensity at spectral line centres will approach the black-body intensity.

Utilising the intensity of the strongest spectral lines, we show that the plasma
55 electron temperature in a capillary discharge plasma can be deduced using the high wavelength Rayleigh-Jeans limit [12] of black-body emission fitted to the most intense spectral line intensities. The diagnostic technique is applicable to determining the electrons temperatures in capillary discharge plasmas at times where significant pinching of the plasma column is not occurring and should be
60 generally useful for measurements of temperatures < 10 eV in uniform plasmas with large optical depth.

3. Experiment

The capillary discharge used was manufactured by ‘XUV lasers’ (see [13]) and is partly described by Heinbuch et al [14]. Emission along the axis of
65 the 0.2 m long, diameter 3 mm capillary discharge plasma passed through a glass window and was imaged onto a fibre optic cable leading to a Maya Ocean Optics spectrometer with dispersion using a 300 lines/mm diffraction grating and a measured spectral resolution of ≈ 1 nm (see figure 1 for a schematic of the experimental set-up). Spectra arising from the argon fill gas and some impurities
70 were recorded and interpreted for the different stages of plasma heating.

The plasma is heated by radio-frequency (RF) waves for a total duration of 1 ms, a small current pre-ionisation pulse over a much shorter time of $\approx 15\mu\text{s}$ after $2 - 4\mu\text{s}$ of RF heating and a large current induced by a driving pulse of 30 - 40 kV stepped up by a Blumlein arrangement to ≈ 0.3 MeV potential

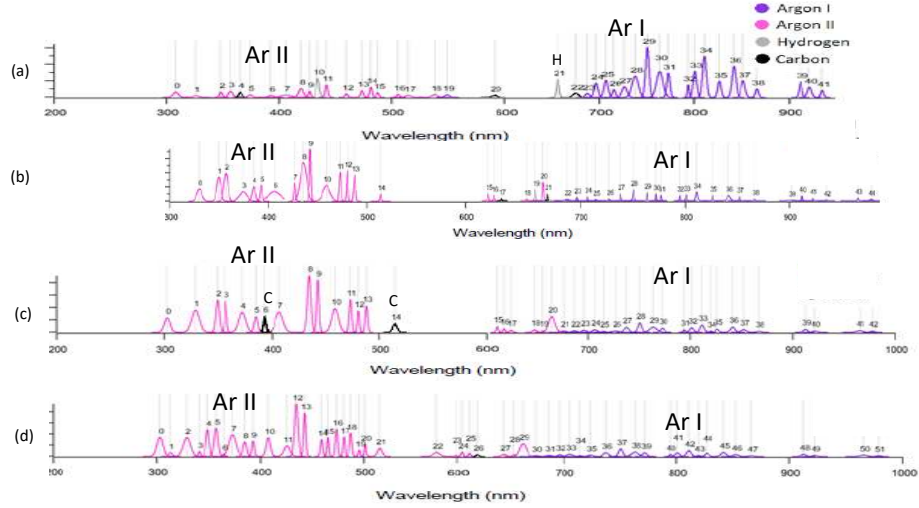


Figure 2: Spectral intensities emitted from the capillary discharge plasma: (a) radio-frequency (RF) heating only, (b) RF heating and a low current pre-ionisation pulse, (c) RF heating, low current pre-ionisation and a high current pulse with driving potential (before Blumlein compression) of 30 kV, (d) as for (c), but with driving potential of 40 kV. The spectral lines are identified as labelled as arising from mainly Ar I or Ar II, with some hydrogen and carbon lines identified.

75 creating a plasma current of 20 - 40 kAmps for $\approx 1\mu\text{s}$ at a time $9\mu\text{s}$ after the start of the pre-ionisation pulse. The high voltage components of the electrical pulse forming network are enclosed in flowing and cooled MIDEAL 1215 organic dielectric fluid. Spectra were recorded with RF heating only, RF heating plus low current pre-ionisation, and RF heating plus low current pre-ionisation plus
 80 high current electrical pulse (figure 2).

Recorded sample spectra are integrated over times (6 ms) longer than the times when plasma exists. The overall temporal plasma emission in the visible can be expected to be largely determined by the RF heating time which is constant for a duration of 1 ms, though significantly increased average ionisation
 85 is observed when there is also an electrical discharge through the plasmas (see figure 2). To aid the identification of lines and the measurement of the intensities of the lines, the continuum emission is removed from the plots shown in figure

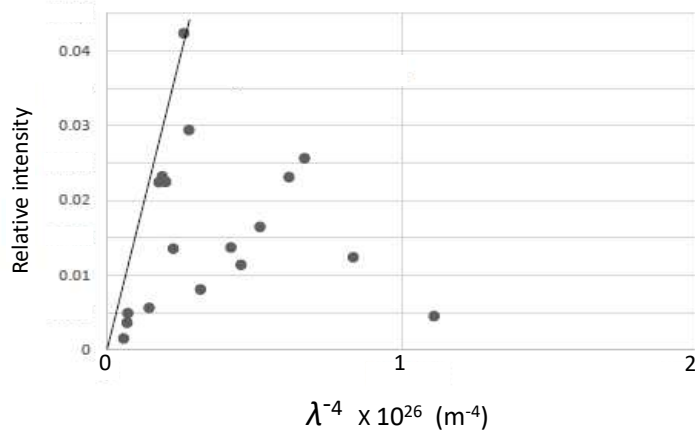


Figure 3: Spectral intensities for different spectral lines emitted from the capillary discharge plasma with a driving potential of 30 kV plotted as a function of the spectral line wavelength λ raised to the power -4. . The black-body emission for a temperature of 1.45 eV is shown as a straight line.

2. Lines are identified in figure 2 as arising from Ar I, Ar II, carbon or hydrogen using the wavelengths listed in the NIST database of spectral lines [15]. A
 90 numbering system and small vertical marker for each spectral line is included in figure 2 as a label. Under the same discharge conditions, the recorded spectral intensities were found to be reproducible for each stage of plasma heating to within 5 percent.

In the high wavelength limit, the Rayleigh-Jeans expression for black-body
 95 intensity I_p for a radiation temperature T at wavelength λ is given by

$$I_p = \frac{2ck_B T}{\lambda^4}. \quad (2)$$

Optical pyrometers use the Rayleigh-Jeans expression [12] to measure temperatures of hot solid objects radiating as black-bodies. However, in plasmas, it is unusual for radiation to interact sufficiently for the radiation to be black-body at all frequencies.

100 Intense spectral lines are the most likely components of the radiation spectrum to interact with matter, and consequently the maximum intensity for a

spectral line approaches the black-body intensity with the radiation temperature equal to the electron temperature. Plotting the intensity I (in relative units per unit wavelength) of different spectral lines emitted from the capillary plasma as a function of $1/\lambda^4$ shows that the maximum intensity for any value of $1/\lambda^4$ is defined by a line corresponding to the maximum allowed value associated with the black-body intensity (see figure 3). The error in assigning the line of maximum intensity in figure 3 produces an error in the deduced relative temperature as shown by the horizontal error bars in figure 4. The error in a relative temperature measurement is not large because there is always an accurate point at zero intensity and zero value of λ^{-4} in plots of the form of figure 3.

An absolute temperature measurement requires an absolute calibration of the intensity I as a function of wavelength λ and was undertaken with the Ocean Optics LS-1-CAL tungsten halogen light source assuming emission occurs for the duration (1 ms) of the RF plasma heating. We used the following procedure to check the calibration of the absolute intensities I . Electron temperatures can be measured from the ratio of the intensity of optically thin spectral lines if the excited state populations are in equilibrium with each other. A Boltzmann ratio of populations causes the intensity I of spectral lines of photon energy E_p with the same final quantum state to vary in temperature T with proportionality such that

$$I \propto E_p g_p A_p \exp\left(-\frac{E_p}{k_B T}\right) \quad (3)$$

where g_p is the degeneracy of the upper quantum state and A_p is the spectral line transition probability [12]. Temperatures deduced in detailed analysis using equation 3 with less intense spectral lines likely to be close to optically thin were found to be in agreement with temperatures measured using equation 2. However, temperatures measured using equation 3 were found to have a greater relative error compared to the calibrated Rayleigh-Jeans method (equation 2) because (i) $E_p < k_B T$ and hence the intensity variation (equation 3) becomes insensitive to temperature for some spectral lines, (ii) there is a remaining un-

certainty that the spectral lines are optically thin and (iii) the intensities of less intense lines are measured with greater relative error compared to the measured intensities of intense spectral lines.

For different discharges with increasing heating, we find that the measured
 135 temperatures increase (see figure 4). The spectral resolution of the spectrometer (≈ 1 nm) was verified as sufficient to resolve the emitted widths of Ar I and Ar II spectral lines. The more intense spectral lines are opacity broadened which ensures that measuring the peak intensity of a spectral line (as for figure 3) records the black-body intensity.

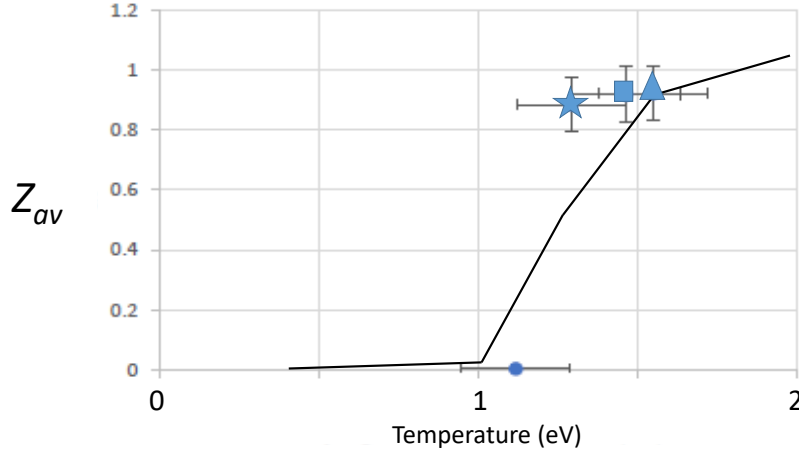


Figure 4: The average ionisation Z_{av} determined from the relative abundance of Ar II and Ar I spectral lines as a function of the temperature measured as described for figure 3. Different heating mechanisms are indicated by different data points (circle: radiofrequency (RF) alone, star: RF and pre-ionisation current, square: RF, pre-ionisation and 30 kV supplied to electrical pulse, triangle: as for the square with 40 kV). The solid curve shows the ionisation calculated with the FLYCHK collisional-radiative code.

140 An estimate of the average ionisation in the capillary discharge plasma was made by summing up the measured intensities of all recorded singly ionised argon (Ar II) emission and the intensities of all neutral argon emission (Ar I). In models of plasma emission [12], these intensities are proportional to the

abundances (n^+ and n) of respectively singly ionised and neutral argon with a
145 similar proportionality constant. We can write for the average ionisation Z_{av}
that

$$Z_{av} = \frac{n^+}{n^+ + n}. \quad (4)$$

The values of average ionisation Z_{av} estimated in this way as a function of the
temperature measured as outlined for figure 3 are shown in figure 4. For com-
parison, the average ionisation Z_{av} as calculated by the collisional-radiative code
150 FLYCHK [16] at densities where coronal equilibrium is applicable is superim-
posed on figure 4. There is good agreement between the measured parameters
and the collisional-radiative prediction (figure 4).

The presence of carbon and hydrogen spectral lines (figure 2) suggests that
there is contamination of the organic dielectric oil in some of the argon plasma
155 discharges. Such contamination can change the resistivity of the plasma and
reduce the effectiveness of the plasma pinch. It is clearly useful to monitor the
optical emission from the plasma to check for impurities and also to measure
the average temperatures of the plasma.

4. Conclusions

160 We have demonstrated a technique for temperature measurement using the
peak intensity of optically thick lines as their intensities approach a black-body
distribution. Recording optical emission in the wavelength range 300 - 1000 nm
from a plasma formed by RF heating and electrical discharges in a 0.2 m long
capillary plasma, we have shown that the high wavelength Rayleigh-Jeans form
165 of the black-body emission can be fitted to the most intense spectral lines to
give a measurement of plasma temperatures in the 1 - 1.5 eV range. Optically
thick spectral line emission from plasmas is often difficult to use for the diagnosis
of plasma parameters and the proposed procedure does not require any detailed
atomic physics knowledge of, for example, transition probabilities. The tem-
170 perature measurement technique should have wider applicability in diagnosing
plasmas with optically thick spectral lines.

Acknowledgements

We thank Professor C. Menoni and Professor J. J. Rocca (Colorado State University) for advice and help running the capillary discharge.

175 References

- [1] Edison, N., Young, P. E., Homes, N. et al (1993) Phys. Rev. E47, 1305.
‘Characterization of a capillary-discharge plasma’.
- [2] Steinhauer, L. C. and Kimura, W. D. (2006) Phys. Rev. Spec. Topics -
Accel. and Beams 9, 081301. ‘Quasistatic capillary discharge plasma model’.
DOI: 10.1103/PhysRevSTAB.9.081301
- [3] Spence, D. J., Butler, A. and Hooker, S.M. (2003) J. Opt.
Soc. Am. 20, 138. ‘Gas-filled capillary discharge waveguides’. DOI:
/10.1364/JOSAB.20.000138
- [4] Kaganovich, D., Ting, A., Moore, C. I. et al (1999) Phys. Rev. E59, R4769.
‘High efficiency guiding of terawatt subpicosecond laser pulses in a capillary
discharge plasma channel’.
- [5] Smirnov, B. M. and Tereshonok, D. V. (2014) Euro. Phys. Lett. 105,
35001. ‘Plasma of capillary discharge of low pressure’. doi: 10.1209/0295-
5075/105/35001
- [6] Avaria, G., Grisham, M., Li, J., Tomasel, F. G., Shlyaptsev, V. N., Busquet,
M., Woolston, M. and Rocca, J. J. (2015) Phys. Rev. Lett. 113, 095001. ‘Ex-
treme degree of ionization in homogenous micro-capillary plasma columns
heated by ultrafast current pulses’.
- [7] Machchietto, C. D., Benware, B. R. and Rocca, J. J. (1999) Optics Lett.
24, 1115. ‘Generation of millijoule-level soft-x-ray laser pulses at a 4- Hz
repetition rate in a highly saturated tabletop capillary discharge amplifier’.
- [8] Rocca, J. J. (1999) Rev. Sci. Instrum. 70, 3799. ‘Table-top soft X-ray lasers’.
- [9] Rossall, A. K., Aslanyan, V., Tallents, G. J., Kuznetsov, I., Rocca, J. J.
and Menoni, C. S. (2015) Phys. Rev. Appl. 3, 064013. ‘Ablation of submi-
crometer holes using an extreme ultraviolet laser’. DOI: 10.1103/PhysRe-
vApplied.3.064013

- [10] Aslanyan, V., Kuznetsov, I., Bravo, H., Woolston, M. R., Rossall, A. K., Menoni, C. S., Rocca, J. J. and Tallents, G. J. (2016). APL Photonics, 1, 066101. ‘Ablation and transmission of thin solid targets irradiated by intense extreme ultraviolet laser radiation’. DOI: 10.1063/1.4953669
- [11] Shlyaptsev, V. N., Dunn, J., Moon, S. J. et al (2002) IEEE 5th Intern. Conf. dense Z-pinches. Ed. David, J et al. ‘Modeling of capillary discharge plasma for x-ray lasers , XUV lithography and other applications’. DOI: 10.1063/1.1531364
- [12] Tallents, G. J. (2018). An introduction to the atomic and radiation physics of plasmas (Cambridge Univ. Press, Cambridge). DOI: 10.1017/9781108303538
- [13] <http://www.xuvlasers.com/welcome.html> (accessed May 23, 2018).
- [14] Heinbuch, S., Grisham, M., Martz, D. and Rocca, J. J. (2005) Optics Express 13,4050. ‘Demonstration of a desk-top size high repetition rate soft x-ray laser’. DOI: 10.1364/OPEX.13.004050
- [15] https://physics.nist.gov/PhysRefData/ASD/lines_form.html (accessed May 24, 2018).
- [16] Chung, H. K., Chen, M. H., Morgan, W. L., Ralchenko, Y. and Lee, R. W. (2005) High Energ. Dens. Phys. 1, 3. ‘Generalized population kinetics and spectral model for rapid spectroscopic analysis for all elements’.