



UNIVERSITY OF LEEDS

This is a repository copy of *Investigation into the validity of WearCompare, a purpose-built software to quantify erosive tooth wear progression*.

White Rose Research Online URL for this paper:
<http://eprints.whiterose.ac.uk/152143/>

Version: Accepted Version

Article:

O'Toole, S, Osnes, C orcid.org/0000-0003-4652-3854, Bartlett, D et al. (1 more author) (2019) Investigation into the validity of WearCompare, a purpose-built software to quantify erosive tooth wear progression. *Dental Materials*, 35 (10). pp. 1408-1414. ISSN 0109-5641

<https://doi.org/10.1016/j.dental.2019.07.023>

Crown Copyright © 2019 Published by Elsevier Inc. on behalf of The Academy of Dental Materials. All rights reserved. This manuscript version is made available under the CC-BY-NC-ND 4.0 license <http://creativecommons.org/licenses/by-nc-nd/4.0/>.

Reuse

This article is distributed under the terms of the Creative Commons Attribution-NonCommercial-NoDerivs (CC BY-NC-ND) licence. This licence only allows you to download this work and share it with others as long as you credit the authors, but you can't change the article in any way or use it commercially. More information and the full terms of the licence here: <https://creativecommons.org/licenses/>

Takedown

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing eprints@whiterose.ac.uk including the URL of the record and the reason for the withdrawal request.



eprints@whiterose.ac.uk
<https://eprints.whiterose.ac.uk/>

Title: Investigation into the validity of WearCompare, a purpose-built software to quantify erosive tooth wear progression

O'Toole S¹, Osnes C^{2,3}, Bartlett D¹, Keeling A².

¹Centre for Clinical, Oral and Translational Sciences

King's College London Faculty for Dental, Oral and Craniofacial Sciences,

Guy's Hospital,

London,

SE1 9RT, UK.

²Department of Restorative Dentistry

School of Dentistry,

University of Leeds,

Leeds,

LS2 9LU, UK.

³Department of Medical Biotechnologies,

University of Siena,

Siena,

Italy

Abstract

Objectives: The use of surface matching software with intraoral scanners is developing rapidly which increases the need for accessible, accurate and validated measurement software. This investigation compared the current gold-standard Geomagic Control software to a purpose-built software “WearCompare”.

Methods: Artificially created occlusal defects of a known size were created on 10 natural molar teeth scanned with a structured-light model-scanner (Rexcan DS2, Europac 3D, Crewe). The volume change, maximum profilometric loss and mean profilometric loss were obtained from both Geomagic Control (3D Systems, Darmstadt, Germany) and WearCompare (leedsdigitaldentistry.com). Duplicated datasets were randomly repositioned and re-alignment performed. The effect of the re-alignment was calculated by analysing differences between the known defect size and defect size after re-alignment using the same measurement metrics. Lastly, clinical wear measurements were compared on natural molar surfaces (n=60) over 6 months using study models collected from a previous longitudinal trial. Data analysis was performed in SPSS v25 (paired t-tests, Pearson correlations, $p < 0.05$).

Results: Measurement correlation between the softwares was greater than 0.97 ($p < 0.001$) for all measurement metrics. The volume change error (SD) after alignment was $-0.67 \text{ mm}^3(1.14)$ for Geomagic and $-0.06 \text{ mm}^3(0.93)$ for WearCompare ($p=0.140$ and $r=0.065$, $p=0.86$). Measurement errors were observed after alignment in both softwares and no statistical differences were observed between softwares. The volume change on the clinical dataset over 6 months was $+0.29 \text{ mm}^3(3.97)$ in Geomagic and $-0.30 \text{ mm}^3(1.82)$ for WearCompare ($p=0.19$ and $r=0.61$, $p < 0.001$). The mean profile gain was $42.86 \text{ }\mu\text{m}(40.19)$ for Geomagic and $32.17 \text{ }\mu\text{m}(23.72)$ for WearCompare ($p=0.048$). Correlations between the softwares were greater than 0.6 for all measurement metrics except for mean profile gain.

Significance: WearCompare is a comparable tool to Geomagic for quantifying erosive tooth wear. WearCompare reported statistically less profile gain indicating less error but further research is needed to reduce the human errors in both softwares.

Introduction:

The use of surface matching software to quantify tooth wear progression is developing rapidly with potential to revolutionise the diagnosis and management of erosive tooth wear. To date, in vivo tooth wear measurement has relied upon visual qualitative assessment of casts of accurate analogue impressions of teeth taken at consecutive appointments [1,2]. Quantitative methods have utilized accurate impressions which are subsequently cast in dental stone [3], epoxy resin [4] or electro-conductive coatings [5] and then scanned, using laboratory based profilometers, and the digital maps aligned using commercial surface matching software or purpose built in-house software [6,7] to calculate differences between them [3,8–11]. This methodology has meant these techniques have been limited to university settings due to the specialised equipment needed for digitising and analyzing the complex tooth surfaces. The rapid and increasing improvement in the trueness and precision of intraoral and model scanners makes it unlikely that digitization of surfaces will be a limitation in the future. This makes the need for an accessible, accurate and validated software to superimpose scans and quantify intraoral changes more pertinent to facilitate accurate diagnosis in primary care.

The accurate superimposition of two scans and measurement of differences is a problem not limited to dental applications. To date, two 3D pointclouds are typically registered using either clusters of data points (features) or by aligning each individual data point, independent of the overall match in shapes. An iterative closest point alignment has been the approach taken by the majority of previous researchers in this area and the known disadvantages of these have been noted [12,13]. However, point registration algorithms are forced to align surfaces in a way that is not biologically informed, which can lead to severe local distortions. Engineering research suggests that a feature-based superimposition produces more accurate results and is less susceptible to outliers [14]. In addition to the technique used to register the two scans, the

accuracy of alignment can be impacted by the areas chosen to align the scans with. A global best fit alignment approach is quick to perform and has been widely used [15,16]. However, this can lead to errors particularly in cases whereby a specific area of interest is anticipated to have changed more than others [17]. For example, in the case of molar occlusal tooth wear, global alignment will act to minimise all inter-surface distances between sequential scans. This has the effect of pulling the worn tooth in an occlusal direction, giving an erroneous underestimate of the amount of tooth wear and in some cases, reporting tooth gain. More accurate measurements can be achieved through selective surface alignment where the operator uses clinical judgement to select reference areas to align with and change is only measured on the surface of interest [17]. Despite the operator influenced error of the system, these principles and other feature-based surface matching algorithms, have been utilised for advanced free-form surface registration on MRI scans [18,19] and other applications [20].

Different methods for analysing differences between surfaces have included maximum surface height loss [11,21], average profile height loss [3,4], volume change [4,8,22] and percentage of surface area affected by wear [5]. Different methods of data extraction may be influenced to differing degrees by the method of alignment [13]. No one methodology has been used consistently and different methods have not been compared to date

The aim of this paper was to investigate the validity of a purpose-built surface matching freeware designed for dental applications. WearCompare (<https://leedsdigitaldentistry.com/wearcompare.html>) is based upon the use of advanced feature-based registration techniques and selective surface alignment. This software was compared to the current gold-standard, widely used Geomagic Control engineering software (3D Systems, Darmstadt, Germany). Our null hypothesis is that there is no difference and strong correlation between measurements taken with both systems.

Materials and Methods

All electronic data used for this study were obtained from a previous longitudinal clinical trial measuring wear on teeth on 60 patients over a 6 month period (O'Toole et al. 2018, REC Ref: 14/EM/1171, clinical trials.gov registration ID: NCT02493803 [10]). Silicone impressions of teeth taken at baseline and 6 months later were poured in type 4 dental stone and the occlusal surfaces of the lower molars scanned using a triangulation laser profilometer (Xyris 2000TL, TaiCaan, Southampton, UK) and data recorded every 50 μm , scanning from left to right in a raster pattern, at medium precision mode (scanning speed of 2.81 mm/s)[3]. This laser is accurate to 1.3 μm and repeatable to 1.6 μm . The coefficient of variation on volume measurements is <5% [23].

Comparison using existing alignment

Initially, ten random baseline scans of the occlusal surfaces of the lower first molars were chosen and a defect of 300 μm in depth was subtracted using Meshlab [24] in accordance with previously published protocols [17]. This created two scans in perfect alignment but with a quantifiable defect size. The differences between the scans were quantified using the gold standard Geomagic Control (3D Systems, Darmstadt, Germany) and with "WearCompare" (<https://leedsdigitaldentistry.com/wearcompare.html>). These differences were; volume change (overall volumetric change in mm^3), mean profile loss (average surface loss measured in microns), maximum point loss (the maximum point of loss recorded over the occlusal surface in microns), mean profile gain (average surface gain measured in microns) and maximum point gain (the maximum point of gain recorded over the occlusal surface in microns).

Comparison using re-alignment

The same scans were duplicated and then randomly repositioned undergoing a random rotation about an axis varying 0–360°, and a displacement along X, Y and Z between –10 and +10 mm. Re-alignment with the baseline scan was then performed using a selective surface technique in both Geomagic Control and WearCompare. Selective surface alignment in Geomagic was performed according to previously published protocols [17] whereby the displaced file was duplicated and area with the defect was removed from the scan and the remaining sections used for alignment. For selective surface alignment in WearCompare, an initial alignment was performed, the defect and reference areas were highlighted and the same measurements taken (Figure 1).

Aligning and measuring a clinical data set.

Lastly, clinical wear using the baseline and after 6 months (n = 30 patients and 60 molars) compare between Geomagic and WearCompare [6]. The scan from each molar (n=60) was aligned using the same selective surface alignment technique as described above in Geomagic and WearCompare and the differences compared.

Results

Comparison using existing alignment

Figure 2 shows the average volume of the defect (SD) measured in Geomagic was 11.83 mm³ (3.46) and 11.86 mm³ (3.61) in Wear Compare (p=0.771) and were highly correlated (0.998, p<0.001). There were high correlations of greater than 0.97 for all measurement metrics with no statistical differences between any measurement metric in Geomagic and WearCompare.

Comparison using re-alignment

The re-alignment showed the volume change error (SD) of -0.67 mm^3 (1.14) for Geomagic and -0.06 mm^3 (0.93) for WearCompare ($p=0.140$ and $r=0.065$, $p=0.86$). Figure 3 reports the measurement metrics for maximum point change errors and mean profile change errors. The average maximum point loss error was $-15.63 \mu\text{m}$ (33.57) and $-18.3\mu\text{m}$ (14.08) respectively. Interestingly, the only measurement metric to be correlated between the two softwares was mean loss error ($r=0.822$, $p=0.004$).

Aligning and measuring a clinical dataset.

The average volume change on 60 molar surfaces over 6 months measured by Geomagic was $+0.29 \text{ mm}^3$ (SD=3.97) and for WearCompare -0.30 mm^3 (SD=1.82). ($p=0.19$ and $r=0.61$, $p<0.001$). Figure 4 reports the mean and maximum loss for Geomagic was $40.32 \mu\text{m}$ and $273.11 \mu\text{m}$ and the mean and maximum profilometric loss for WearCompare was $37.37 \mu\text{m}$ and $247.87 \mu\text{m}$ ($p >0.05$). The maximum gain for Geomagic was $215.09 \mu\text{m}$ (SD 132.78) and WearCompare $184.39 \mu\text{m}$ (SD 126.06) and these were statistically different ($p=0.015$) and values were correlated ($r=0.623$, $p<0.001$). The mean profile gain for Geomagic was $42.86 \mu\text{m}$ (SD 40.19) and for WearCompare $32.17 \mu\text{m}$ (SD 23.72) and was statistically different ($p=0.048$) but moderately correlated ($r=0.523$ $p<0.001$) and Figure 5.

Discussion

A very high correlation was observed between Geomagic and WearCompare when quantifying the same defect, indicating that measurements from either software are equally valid. However, the measurements were not strongly correlated after re-alignment, despite the fact that there were no statistical differences between the values observed. This indicates that there were

differences in the alignment algorithm. Differences between the softwares were also observed in the clinical data and therefore the null hypothesis was rejected.

There are several reasons for differences between the softwares. Firstly, the underlying surface registration algorithm is different. WearCompare uses a feature based global registration [25] coupled with a custom iteratively refined version of the Iterative Closest Point algorithm [26]. This contrasts with Geomagic which uses a variation of an Iterative Closest Point algorithm alone to align corresponding points in the 3D dataset with greater potential to skew the data. This may explain why WearCompare reported significantly less positive deviation error or “gain” than Geomagic using the clinical dataset. Secondly, there is a difference in how the two softwares handle peripheral data. Ideally data located at the periphery of the scan needs to be removed to obtain two coincident scan sizes. In Geomagic, unless a plane is used to section through the 3D mesh, the accuracy of the periphery of the mesh is limited to the size of the triangle which is typically 50 microns but can go up to 100-200 microns [27]. WearCompare automatically sections through triangles. A third reason is differences between the handling of voids in scan. If a void is not filled by the operator, Geomagic will analyse this data as part of the scan. WearCompare automatically fills in voids following the curvature when taking measurements.

The most appropriate measurement metric to quantify tooth wear progression is unknown. Positive gain during alignment represents error in the process. Volumetric change gives an indication of the total surface change [17,28], taking into account negative and positive deviations. In our data, there were no statistical differences in volume change between the two softwares, although the error value was smaller for WearCompare. For the other parameters, mean profilometric loss was consistent between the two softwares and may be the best metric

to use if consistency between the softwares is desired. However, this does mean that all positive data within the alignment is unaccounted for.

Although it does not affect the data, there were differences in the workflow. In Geomagic, using a reference surface alignment requires additional steps and while surface deviations were measured together alongside the colour map, volume calculation requires a separate procedure. In WearCompare all measurement metrics and colour maps are produced simultaneously, reducing the time taken for workflow. This becomes significant when attempting to analyse large numbers for clinical trials. Despite these advancements, there still remains little difference between the softwares. This indicates that the manual process of selective surface alignment requires further development for both accuracy and speed. It worth considering that Geomagic has several other functionalities which may be useful for the advanced user but may add complexity and introduce error for the less advanced user.

There are several limitations of this study. Standard deviations were high for all measurements and indicates the complexity of the surface and the scope for operator error. This may be a reason for the lack of statistical difference between softwares, particularly when determining the alignment errors. There is potential for this to be improved with automation of the process. However, at present, operator error remains a significant limitation of the quantification process. For the third part of the study, data from a previously published clinical study were used to quantify change. There were errors with both systems and it is difficult to assess which was more accurate. It is highly unlikely that tooth tissue gain occurred over the 6 month period and is likely to represent error as a direct and known consequence of the alignment mathematics. WearCompare reported statistically less gain than Geomagic. Despite this limitation, it is promising to note that the two softwares were moderate-highly correlated.

For both softwares, understanding the underlying digital process and errors of the system is important to prevent misinterpretation. An understanding of how to read and apply the results is important, in addition to making the subjective decision that the alignment has not been successful and clinical data cannot be used. Bearing these limitations in mind, it appears that WearCompare is a suitable freeware alternative to Geomagic for the purpose of quantifying tooth wear progression. The speed of use is particularly convenient for researchers wishing to analyse large datasets, while the lack of cost makes WearCompare accessible to the general dentist wishing to monitor individual patients for tooth wear progression. Geomagic may be more suitable for advanced users who seek to use the additional functionality of the software. There are other potential applications with both softwares such as quantifying soft tissue changes following periodontal therapy or surgery which would require further validation.

Conclusion

WearCompare is a suitable freeware tool for quantifying erosive tooth wear and comparable to the previous gold-standard Geomagic software. Although WearCompare reported statistically less gain on the clinical dataset, there are errors regardless of the software used. Further research is needed to reduce the human errors associated with the alignment process to enable confident quantification of wear progression.

References


- [1] Vervoorn-Vis GMGJ, Wetselaar P, Koutris M, Visscher CM, Evälahti M, Ahlberg J, et al. Assessment of the progression of tooth wear on dental casts. *J Oral Rehabil* 2015;42:600–4. doi:10.1111/joor.12292.
- [2] Bartlett DW, Palmer I, Shah P. An audit of study casts used to monitor tooth wear in general practice. *Br Dent J* 2005;199:143–5. doi:10.1038/sj.bdj.4812570.

- [3] Rodriguez JM, Austin RS, Bartlett DW. In vivo measurements of tooth wear over 12 months. *Caries Res* 2012;46:9–15. doi:10.1159/000334786.
- [4] Pintado MR, Anderson GC, DeLong R, Douglas WH. Variation in tooth wear in young adults over a two-year period. *J Prosthet Dent* 1997;77:313–20.
- [5] Chadwick RG, Mitchell HL, Manton SL, Ward S, Ogston S, Brown R. Maxillary incisor palatal erosion: no correlation with dietary variables? *J Clin Pediatr Dent* 2005;29:157–64.
- [6] Mitchell HL, Chadwick RG. Mathematical shape matching as a tool in tooth wear assessment--development and conduct. *J Oral Rehabil* 1998;25:921–8.
- [7] DeLong R, Pintado M, Douglas WH. Measurement of change in surface contour by computer graphics. *Dent Mater* 1985;1:27–30. doi:10.1016/S0109-5641(85)80061-0.
- [8] Tantbirojn D, Pintado MR, Versluis A, Dunn C, DeLong R. Quantitative analysis of tooth surface loss associated with gastroesophageal reflux disease. *J Am Dent Assoc* 2012;143:278–85. doi:10.14219/jada.archive.2012.0153.
- [9] Lambrechts P, Vanherle G, Vuylsteke M, Davidson CL. Quantitative evaluation of the wear resistance of posterior dental restorations: a new three-dimensional measuring technique. *J Dent* 1984;12:252–67. doi:10.1016/0300-5712(84)90071-X.
- [10] O’Toole S, Newton T, Moazzez R, Hasan A, Bartlett D. Randomised Controlled Clinical Trial Investigating the Impact of Implementation Planning on Behaviour Related to the Diet. *Sci Rep* 2018;8:8024. doi:10.1038/s41598-018-26418-0.
- [11] Ahmed K, Whitters CJ, Xiangyang J, Stephen G, MacLeod C, Murray C. Clinical monitoring of tooth wear progression in patients over a period of one year using CAD/CAM. *Int J Prosthodont* 2016;30:153–5. doi:10.11607/ijp.4990.
- [12] Chadwick RG, Mitchell HL, Ward S. Evaluation of the accuracy and reproducibility of a replication technique for the manufacture of electroconductive replicas for use in

- quantitative clinical dental wear studies. *J Oral Rehabil* 2002;29:540–5.
doi:10.1046/j.1365-2842.2002.00894.x.
- [13] Mitchell HL, Koch I, Chadwick RG. Linear interpolation error in measured surfaces in a dental erosion study. *Med Biol Eng Comput* 2004;42:100–5.
doi:10.1007/BF02351017.
- [14] Ren MJ, Cheung CF, Kong LB, Jiang X. Invariant-feature-pattern-based form characterization for the measurement of ultraprecision freeform surfaces. *IEEE Trans Instrum Meas* 2012;61:963–73. doi:10.1109/TIM.2011.2173047.
- [15] Wulfman C, Koenig V, Mainjot AK. Wear measurement of dental tissues and materials in clinical studies: A systematic review. *Dent Mater* 2018;https://doi:10.1016/j.dental.2018.03.002.
- [16] Beuer F, Güth J-F, Edelhoff D, Runkel C, Stimmelmayer M, Keul C. Accuracy of five intraoral scanners compared to indirect digitalization. *Clin Oral Investig* 2016;21:1445–55. doi:10.1007/s00784-016-1902-4.
- [17] O’Toole S, Osnes C, Bartlett D, Keeling A. Investigation into the accuracy and measurement methods of sequential 3D dental scan alignment. *Dent Mater* 2019. doi:10.1016/j.dental.2019.01.012.
- [18] Xue N, Doellinger M, Fripp J, Ho CP, Surowiec RK, Schwarz R. Automatic model-based semantic registration of multimodal MRI knee data. *J Magn Reson Imaging* 2015. doi:10.1002/jmri.24609.
- [19] Robinson EC, Jbabdi S, Glasser MF, Andersson J, Burgess GC, Harms MP, et al. MSM: A new flexible framework for multimodal surface matching. *Neuroimage* 2014;100:414–26. doi:10.1016/j.neuroimage.2014.05.069.
- [20] Kong LB, Ren MJ, Xu M. Development of data registration and fusion methods for measurement of ultra-precision freeform surfaces. *Sensors (Switzerland)* 2017;17.

doi:10.3390/s17051110.

- [21] Lambrechts P, Braem M, Vuylsteke-Wauters M, Vanherle G. Quantitative in vivo wear of human enamel. *J Dent Res* 1989;68:1752–4.
- [22] O’Toole S, Newton JT, Hasan A, Moazzez R, Bartlett D. Randomised Controlled Clinical Trial Investigating the Effect of Implementation Planning on Behaviour Related to the Diet. Under Rev [Presented IADR San Fr 2017] 2018.
- [23] Rodriguez JM, Austin RS, Bartlett DW. A method to evaluate profilometric tooth wear measurements. *Dent Mater* 2012;28:245–51. doi:10.1016/j.dental.2011.10.002.
- [24] Cignoni P, Callieri M, Corsini M. Meshlab: an open-source mesh processing tool. 2008:http://www.academia.edu/download/41716786/MeshLab_.
- [25] Zhou QY, Park J, Koltun V. Fast global registration. *Lect. Notes Comput. Sci.*, vol. 9906 LNCS, Springer, Cham; 2016, p. 766–82. doi:10.1007/978-3-319-46475-6_47.
- [26] Besl P, McKay N. A Method for Registration of 3-D Shapes. *IEEE Trans Pattern Anal Mach Intell* 1992;14:239–56. doi:10.1109/34.121791.
- [27] Richert R, Goujat A, Venet L, Viguie G, Viennot S, Robinson P, et al. Intraoral Scanner Technologies: A Review to Make a Successful Impression. *J Healthc Eng* 2017;2017:8427595. doi:10.1155/2017/8427595.
- [28] Fleming GJP, Reilly E, Dowling AH, Addison O. Data acquisition variability using profilometry to produce accurate mean total volumetric wear and mean maximum wear depth measurements for the OHSU oral wear simulator. *Dent Mater* 2016;32:e176–84. doi:10.1016/j.dental.2016.05.004.

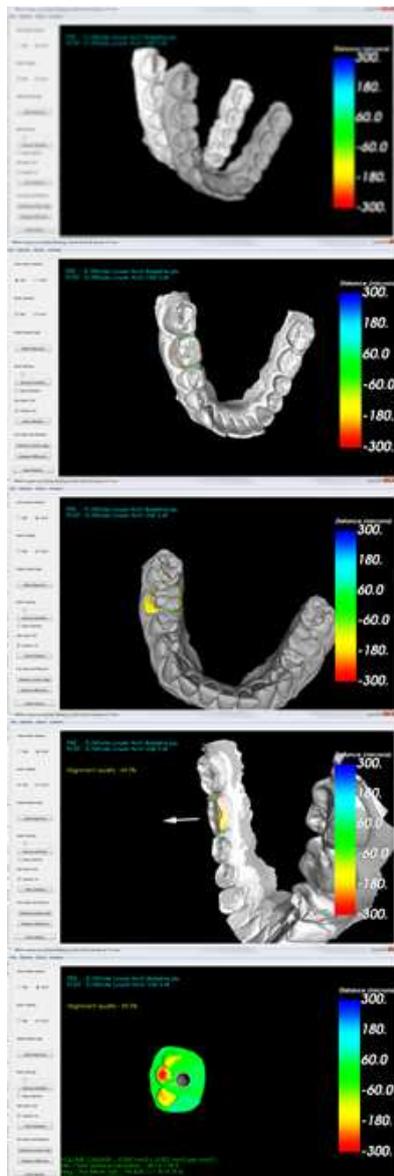

1.1 Two scans taken at separate time points

1.2 Initial alignment followed by manually selecting the measurement surface

1.3 Manual selection of points for alignment (yellow area)

1.4 Selective surface align and choose direction of measurement

1.5 Differences between the two scans are shown in the bottom left corner. Areas in red show areas of wear

Figure 1. Workflow of alignment and measurement with WearCompare

	Average Defect Size in Geomagic (SD)	Average Defect Size in Wear Compare (SD)	Paired Samples T-test	Pearson Correlations
Volume (mm³)	11.83 mm ³ (3.46)	11.86 mm ³ (3.61)	p=0.771	0.998 p<0.001
Maximum Point Loss (µm)	305.36 µm (37.03)	302.53 µm (34.68)	p=0.343	0.971 p<0.001
Maximum Point Gain (µm)	206.56 µm (11.47)	206.68 µm (11.36)	p=0.133	1.000 p<0.001
Mean Profile Loss (µm)	214.13 µm (80.53)	219.61 µm (87.93)	p=0.343	0.983 p<0.001
Mean Profile Gain (µm)	16.12 µm (4.11)	16.29 µm (4.20)	p=0.376	0.991 p<0.001

Figure 2. Correlation between software measurements when quantifying the same defect (n=10)

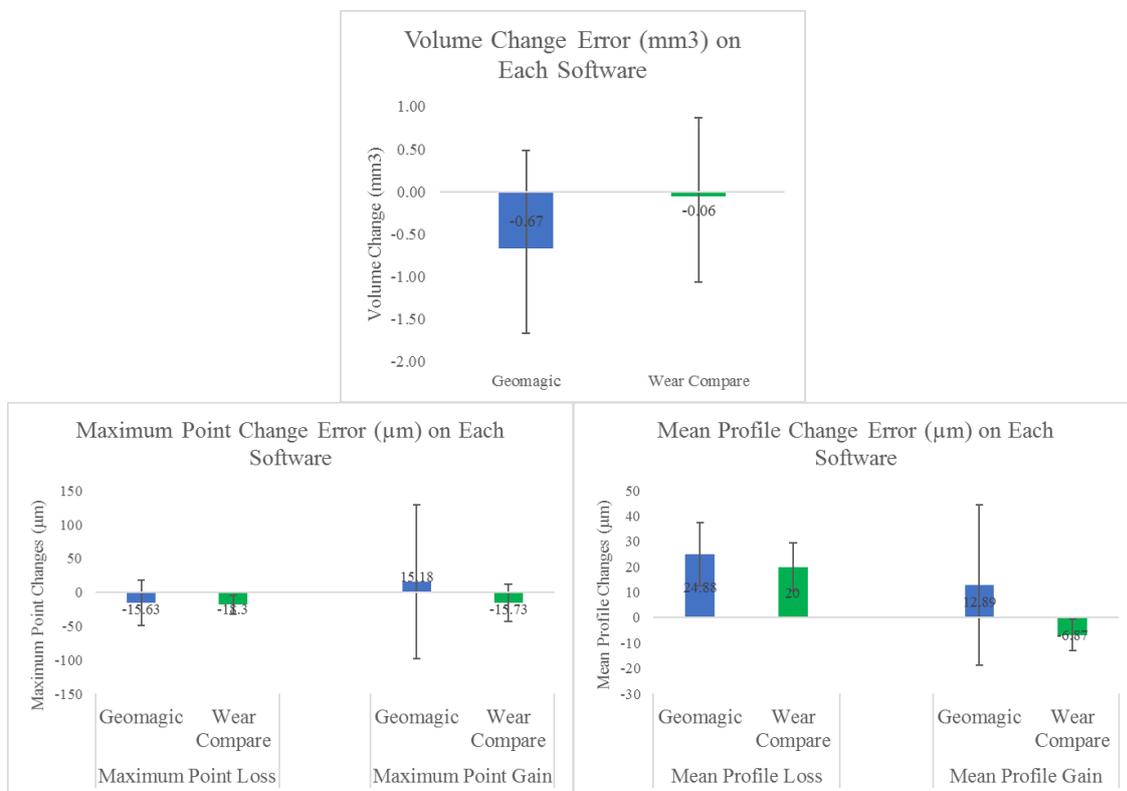


Figure 3. Measurement error in each software when quantifying the same defect after alignment (n=10).

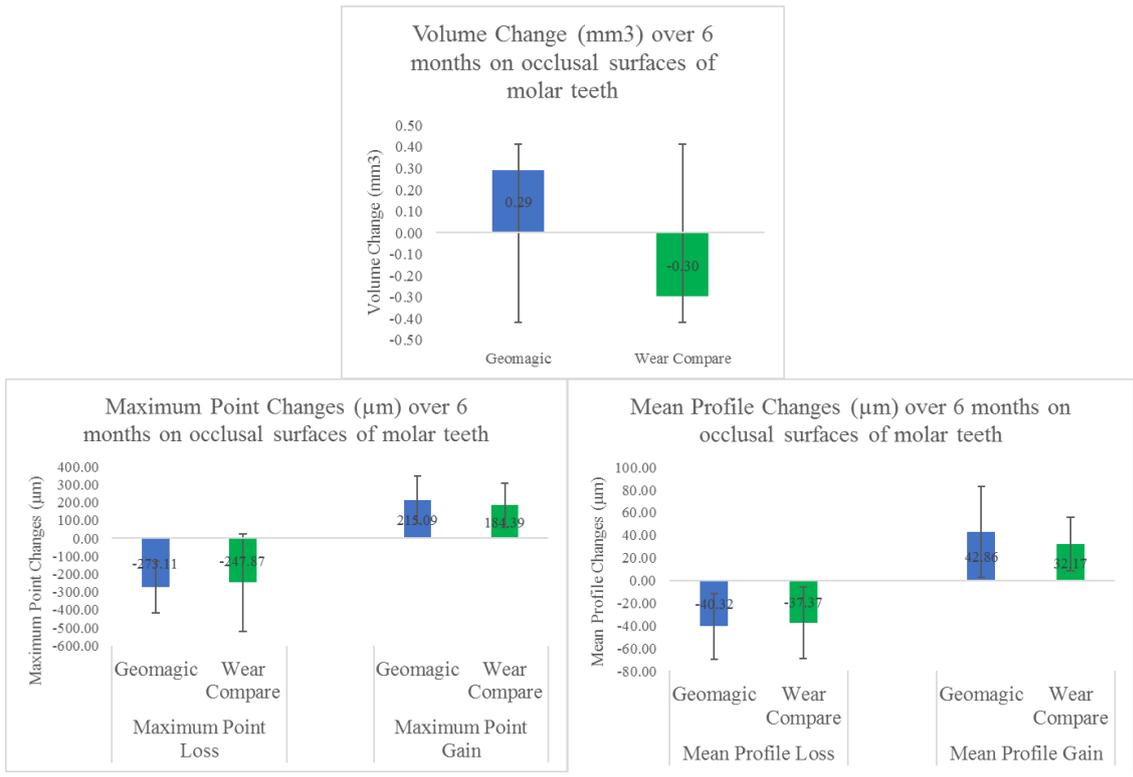


Figure 4. Graphs comparing the changes observed on the occlusal surfaces of 60 molar teeth from 30 patients over a 6-month period when using each software.

	Paired Samples T-test	Pearson Correlations
Volume (mm³)	p=0.194	0.607 p<0.001
Maximum Point Loss (µm)	p=0.516	0.623 p<0.001
Maximum Point Gain (µm)	p=0.015	0.765 p<0.001
Mean Profile Loss (µm)	p=0.412	0.678 p<0.001
Mean Profile Gain (µm)	p=0.048	0.523 p<0.001

Figure 5. Correlation between softwares when quantifying clinical tooth wear progression over 6 months (n=60)