



UNIVERSITY OF LEEDS

This is a repository copy of *Design and control of soft rehabilitation robots actuated by pneumatic muscles: State of the art.*

White Rose Research Online URL for this paper:
<https://eprints.whiterose.ac.uk/165301/>

Version: Accepted Version

Article:

Liu, Q, Zuo, J, Zhu, C et al. (1 more author) (2020) Design and control of soft rehabilitation robots actuated by pneumatic muscles: State of the art. *Future Generation Computer Systems*, 113. pp. 620-634. ISSN 0167-739X

<https://doi.org/10.1016/j.future.2020.06.046>

© 2020, Elsevier. This manuscript version is made available under the CC-BY-NC-ND 4.0 license <http://creativecommons.org/licenses/by-nc-nd/4.0/>.

Reuse

This article is distributed under the terms of the Creative Commons Attribution-NonCommercial-NoDerivs (CC BY-NC-ND) licence. This licence only allows you to download this work and share it with others as long as you credit the authors, but you can't change the article in any way or use it commercially. More information and the full terms of the licence here: <https://creativecommons.org/licenses/>

Takedown

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing eprints@whiterose.ac.uk including the URL of the record and the reason for the withdrawal request.



eprints@whiterose.ac.uk
<https://eprints.whiterose.ac.uk/>

Design and Control of Soft Rehabilitation Robots Actuated by Pneumatic Muscles: State of the Art

Quan Liu, Jie Zuo, Chang Zhu, and Sheng Quan Xie

Abstract— Robot-assisted rehabilitation has become a new mainstream trend for the treatment of stroke patients with movement disability. Pneumatic muscle (PM) is one of the most promising actuators for rehabilitation robots, due to its inherent compliance and safety features. In this paper, we conduct a systematic review on the soft rehabilitation robots driven by pneumatic muscles. This review discusses up to date mechanical structures and control strategies for PMs-actuated rehabilitation robots. A variety of state-of-the-art soft rehabilitation robots are classified and reviewed according to the actuation configurations. Special attentions are paid to control strategies under different mechanical designs, with advanced control approaches to overcome PM’s highly nonlinear and time-varying behaviors and to enhance the adaptability to different patients. Finally, we analyze and highlight the current research gaps and the future directions in this field, which is potential for providing a reliable guidance on the development of advanced soft rehabilitation robots.

Index Terms—Mechanical structure, Control strategy, Pneumatic muscle (PM), Rehabilitation robot

I. INTRODUCTION

IN recent years, the number of stroke patients has increased rapidly and stroke has become the second leading causes of disability [1]. There are about 0.795 million people with stroke in the United States, among them 0.61 million are first or new strokes [2]. In developing countries, the incidence of stroke is even higher. For example, there are 1.3 million new stroke patients every year and three-quarters of them live with motion disability in China. In Latin America, the Middle East, and sub-Saharan Africa,

Research supported by Research supported by National Natural Science Foundation of China under grant numbers 51705381 and 51675389 and the Key Program for International S&T Cooperation of Hubei Province under 2018AHB007, also supported by the UK EPSRC Standard Research Scheme EP/S019219/1. *Corresponding author: Jie Zuo.*

Q. Liu, J. Zuo, and C. Zhu are with the School of Information Engineering, Wuhan University of Technology, Wuhan 430070 China (e-mail: {quanliu, zuojie, changzhu}@whut.edu.cn).

S. Q. Xie is with the School of Electrical and Electronic Engineering, University of Leeds, Leeds LS2 9JT UK (e-mail: s.q.xie@leeds.ac.uk).

there will be a tripling in stroke mortality for the next two decades, one of the major disabled survivors[1]. As a result, the growth of hospitalization rates and prolonged treatment causes a steep increase in the requirement of health care resources. Rehabilitation robotics, which is able to provide robotic assistance for rehabilitation clinics and release the shortage of professional labor-force, has attracted increasing attention in both industrial and academic fields. The rehabilitation robot can assist patients during rehabilitation to restore some of the lost functions. Two kinds of robotic devices are currently available for rehabilitation: end effector robots and exoskeleton robots. Among these studies, PMs become a promising choice in actuators for wearable and compliant rehabilitation devices, due to its high power-to-weight ratios, inherent compliance, and similar behavior with human muscles. In recent years, there have been several well-known PMs-actuated rehabilitation robots, such as the series of upper limb exoskeleton RUPERT [3-5] and lower limb orthosis KAFO [6, 7]. Compared with widely-adopted rigid actuator-type rehabilitation robots, like Lokomat [8, 9] and ArmeoPower [10, 11], there exists no mature PMs-actuated products in the market up to now. Further, the PM's high-nonlinear and time-varying behavior arise the control difficulties for the PMs-actuated robots. "McKibben" muscle is a typical PM, with a cylinder elastic tube and a double helical braid wrapped around the outside, which has been widely utilized in recent soft rehabilitation robots [12]. However, "McKibben" muscle's reticular fiber structure exactly limits its contraction ratio and output force. Hence, some researchers designed straight-fiber- type pneumatic muscles to increase its output force and reduce the friction. Saikawa *et al.* applied high-intensity longitudinal reinforced Kevlar fibers outside the silicone tube to relieve the pneumatic muscle's friction and hysteresis, but it is easy to crack [13]. Likewise, Hirano *et al.* proposed a similar straight- fiber-type artificial muscle [14, 15]. In addition, Beyl *et al.* designed a kind of novel pleated pneumatic artificial muscle (PPM) to drive a powered knee exoskeleton (KNEXO) [16, 17]. Compared with "McKibben" muscle, PPM has a higher threshold pressure and substantial hysteresis [18, 19]. This paper aims to review the remarkable mechanical designs and control strategies of the PMs-actuated rehabilitation robots, targeting to provide valuable information for relevant researcher's further studies.

In the past decade, the application of PMs in rehabilitation robotics has experienced rapid evolution, however, only a few review articles focus on PMs-actuated rehabilitation robots. Andrikopoulos *et al.* summarized the key enabling applications of PMs in various fields, such as biorobotic, medical, industrial and aerospace fields [18]. This review covered most application scenarios of PM, but little details of dynamic models and control strategies are presented. Chou *et al.* classified and discussed PM actuators and high-level control strategies for lower limb wearable robots [19]. But this paper lacks detailed discussion on PM-actuated rehabilitation robots. Additionally, study [20] provides a review on actuating technologies and applications towards wearable robotic orthosis, including electric/hydraulic/ pneumatic actuators, and other promising actuating technologies. Tondu reviewed the modelling methods of "McKibben" muscle [21]. Meng *et al.* discussed mechanisms and control strategies of some PM-driven lower limb rehabilitation robots [22]. Dzahir *et al.* clarified existing applications and control strategies of PMs-actuated lower-limb leg orthoses, but only focusing on the PM antagonistic configurations [23]. As the aspect of control, Andrea *et al.* conducted the

survey on the compliant control approaches for stiff and fixed-compliance robots, especially to promote human-robot interaction [24]. And Young *et al.* provided a complete and informative introduction about the recent development and future direction of the lower limb robotic exoskeleton [25]. Peng *et al.* has published a review article on soft robot with hybrid actuating technology [20]. To the authors' best knowledge, there has not been a review including both design and control of PMs-actuated rehabilitation robots. In particular, the all-round comparisons of existing rehabilitation robots are based on the published available data, to make researchers fully aware of the limitations and advantages of diverse mechanical designs and control schemes. This paper will tell the current research gaps and future directions, promoting the advent of more compliant, adaptable, intelligent and mature robots to satisfy the sharply increasing rehabilitation demands. The rest of paper is organized as follows. Section II clarifies rehabilitation robots with various mechanical structures. In Section III, introduction and comparisons of control strategies are conducted. Section IIV discusses and analyses the research limitations and future directions. Finally, conclusions are drawn in Section V.

II. MECHANICAL DESIGN OF PMS-ACTUTUATED REHABILITAION ROBOTS

A PM mainly contains a braid-covered rubber tube and two closed ends. One end is usually connected to the proportional solenoid valves to regulate the pressure inside the PM, while the other exerts axial-direction contractile force [21]. As a single direction-acting element, the PM can only contract to generate pulling force. To achieve the actuated movements in multiple degree of freedoms (DOFs), PMs are always designed to work together in antagonistic, parallel or bio-inspired configurations.

A. Antagonistic Pair-Based Robots

Antagonistic configuration, as one of the most frequently used actuation schemes, can provide the bidirectional assistance to the patient's joints. One PM antagonistic pair consists of two PMs connected through a cable and a pulley. By regulating the pressure inside each PM, the configuration can provide one rotational DOF assistance. Hence PM antagonistic pairs are widely utilized in upper/lower limb multi-joint exoskeletons and to help patients to complete the assigned movement tasks.

In 2002, University of Salford, UK developed a 7-DOF upper limb rehabilitation exoskeleton actuated by PM antagonistic pairs, as presented in Fig.1(a) [22, 23]. Huazhong University of Science and Technology, China, designed a 9-DOF arm rehabilitation robot fixed to a wheelchair (Fig.1 (b)) [24]. In this device, each active DOF is driven by a PM antagonistic pair. Afterwards, the team developed a novel antagonistic configuration, in which a PM is arranged in place of bicep and the torsion spring provides opposing torque [25, 26]. Jiang *et al.* developed a 4-DOF upper limb rehabilitation robot to provide sufficient rehabilitation assistance for patients with upper limb motion dysfunctions (Fig.1 (c)) [27]. Recently, an exoskeleton for elbow joint rehabilitation was proposed by Tang *et al.* (Fig.1 (d)) [28]. This robot employs four size-adjustable carbon fibers to make subjects more comfortable. However, the air supply equipment is too heavy to allow subject wearing the exoskeleton to complete long-term ground training. Guo *et al.* introduced a joint motion radius element in 1-DOF rehabilitation robot so that the device can be adjusted

to provide the required range of motion and multi-joint progressive assistance for different patient during the whole rehabilitation process[29], as shown in Fig.1 (e). Meng *et al.* designed a wrist exoskeleton, aimed at providing 1-DOF assistance for the patient's wrist rehabilitation (Fig.1 (f)) [30]. A novel modular shoulder exoskeleton was introduced in [31], as shown in Fig.1 (g). The exoskeleton was driven by a modular PM exoskeletal joint and can provide assistance for the patient's whole arm. Then the research team designed a modified Nested-cylinder PMs (NcPAMs), which is more powerful.

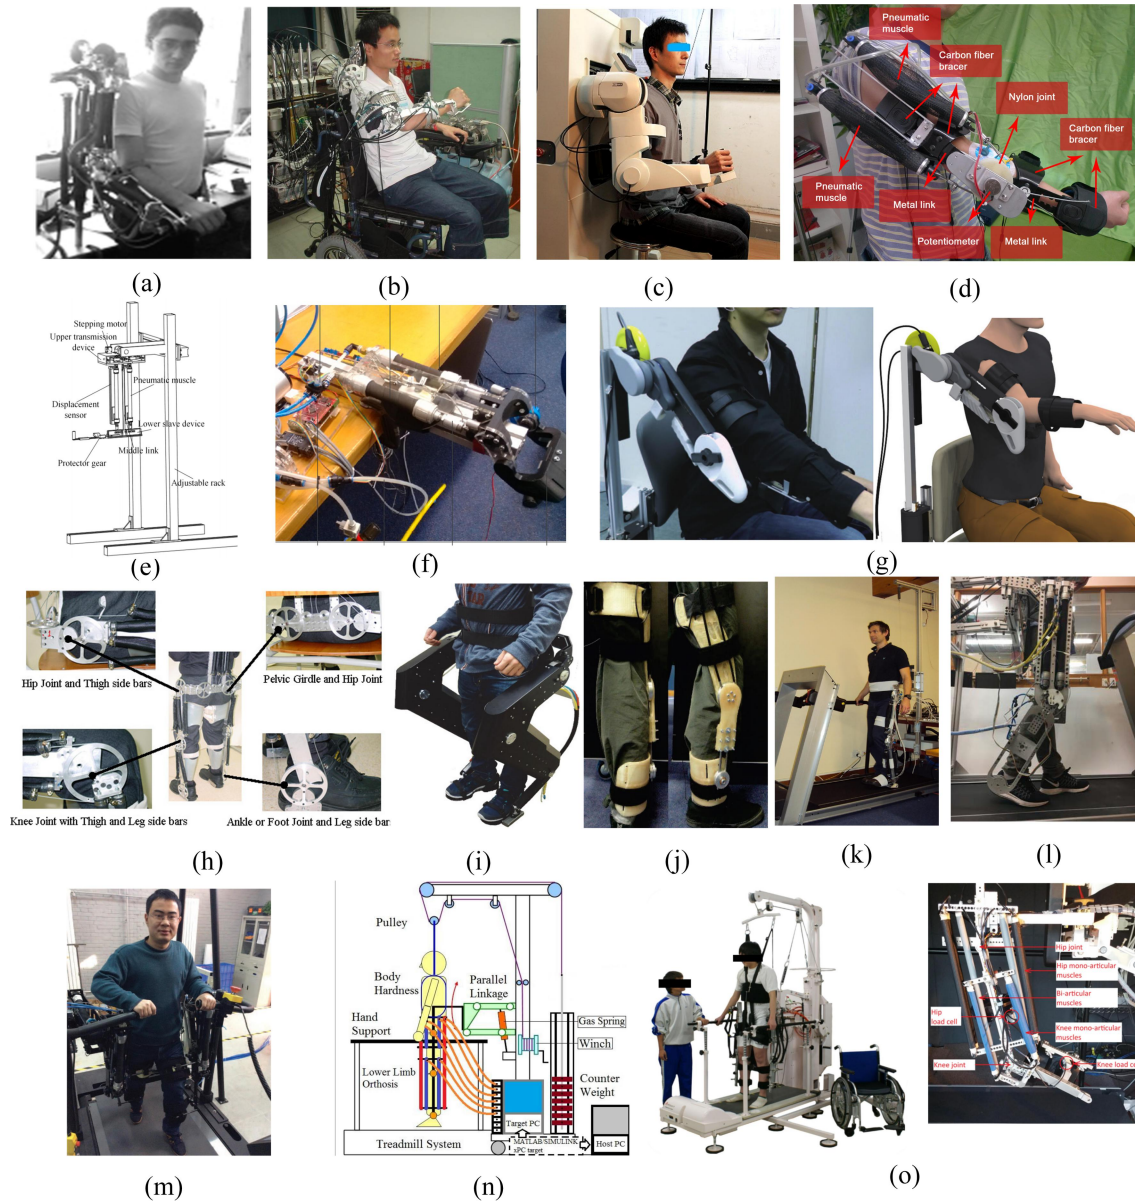


Fig.1. Antagonistic pair-type rehabilitation robots. (a-l) is reprinted from [22, 24, 27-38], respectively.

As for lower limb rehabilitation, antagonistic pair-based exoskeletons are mainly designed to provide walk power assistance. In terms of training modes, the robots can be classified as over-ground exoskeletons and treadmill-based orthoses, both can help to restructure the patient's walking ability. In 2007, Caldwell *et al.* developed a whole-body exoskeleton with seven DOFs for the upper limbs and five DOFs for each of the lower limbs (Fig.1 (h)) [32, 39]. But the output force is too weak to be used in practice.

Kanno *et al* proposed a novel PMs-actuated walking assistive exoskeleton, as presented in Fig.1(i) [33]. Users do not need to adjust the link length of the exoskeleton to fix their knees. HuREx, a human-inspired robotic exoskeleton, was designed for lower limb rehabilitation (Fig.1 (j)) [34]. To reduce the complexity and weight, the exoskeleton was manufactured by 3D printing and fiber reinforcement technologies [40]. Afterwards, the team developed a robotic orthosis for treadmill gait training (Fig.1 (k)) [35, 41]. This orthosis provides trunk's vertical/lateral translation and the hip's passive abduction/adduction assistance for human subjects when walking on the treadmill. The hip and knee sagittal plane rotation torques are produced by PM antagonistic pairs [42]. But it can only be used for the left leg, and the maximum trajectory tracking error is up to 10° . Recently, a modified design has been published, as presented in Fig.1(l) [36]. The knee joint is actuated by a PM antagonistic pair, and each side contains two PMs, to increase the torque and motion range of the joint. Recently, Huang *et al.* presented a treadmill-based gait robotic orthosis actuated by PM antagonistic pairs, as shown in Fig.1(m) [37, 43]. Inspired by the human musculoskeletal system during walking, Dzahir *et al.* developed a gait system (AIRGAIT) powered by antagonistic mono-articular and bi-articular PM actuators (Fig.1 (n)) [38, 44, 45] with larger assistance output. This high compliant lower limb rehabilitation orthosis is aimed to guide the patient's lower-limb to a designate trajectory and can adapt the compliance according to the patient's disability [46, 47], as shown in Fig.1 (o).

TABLE I
OVERVIEW OF ANTAGONISTIC PAIR-BASED ROBOTS

Robots	Aims	Actuated DOFs	Assistance capacity	References
Upper limb exoskeleton	Helping the disabled to achieve natural motion from shoulder to the wrist	7-DOF: shoulder FE/AA, elbow FE/SP, wrist FE/AA	Approximately 20% of ROHIS	Caldwell <i>et al.</i> [22, 23]
Arm rehabilitation robot	Recovering motor function for stroke patients	9-DOF: shoulder FE/AA/LM, elbow FE/SP, wrist FE/AA	73%~91% of ROHM	Jiang <i>et al.</i> [24-26]
Upper limb rehabilitation robot	Providing assistance for patients with upper limb motion dysfunctions	4-DOF: three active DOFs and one passive DOF	--	Jiang <i>et al.</i> [27]
Upper-limb power-assist exoskeleton	Developed to assist physically disabled or elderly people	1-DOF: elbow FE	ROM of $0\sim 180^\circ$ and $0\sim 145^\circ$ for shoulder/ elbow, respectively	Tang <i>et al.</i> [28]
Multi-joint Progressive rehabilitation robot	Providing the required range of motion and multi-joint progressive assistance	1-DOF: can be adjusted to assist knee, elbow, shoulder joint	ROM of knee, elbow, shoulder joint with $\pm 70^\circ$, $\pm 55^\circ$ and $\pm 40^\circ$	Guo <i>et al.</i> [29]
Modular shoulder exoskeleton	Designed to assist the patient's shoulder and whole arm	1 DOF: shoulder FE	Nominal maximum torque is 45 Nm	Noda <i>et al.</i> [31]
Wrist rehabilitation robotic device	Assisting the stroke and cerebral palsy patients to achieve wrist rehabilitation exercise	1-DOF: wrist FE	ROM of up to $-30^\circ\sim 30^\circ$ and the maximum force output up to about 60 N	Meng <i>et al.</i> [30]
Whole-body exoskeleton	Designed for limb retraining, rehabilitation and power assistance	17-DOF: shoulder FE/AA/LM, elbow FE/SP, wrist FE/AA, hip FE/AA/LM, knee FE, ankle DP	$>41\%$ of ROHM and $>86.4\%$ of ROHIS	Caldwell <i>et al.</i> [32, 39]
Treadmill-based gait training robotic orthosis	Helping stroke patients to regain mobility	2-DOF: hip FE, knee FE	ROM of $0\sim 85^\circ\sim 25^\circ$ and ROT of 40/60 Nm for knee/hip joint	Huang <i>et al.</i> [37, 43]
Lower limb robotic orthosis	Providing treadmill training of neurologically impaired subjects	2-DOF: hip FE, knee FE	ROM of $60^\circ/30^\circ$ and $90^\circ/30^\circ$ for hip/knee	Hussain <i>et al.</i> [36]
Walking assist device	Assisting patients with performance of walking	1-DOF: knee FE	ROM of $-3\sim 93^\circ$	Cao <i>et al.</i> [35, 41]
Human-inspired robotic exoskeleton (HuREx)	Developed for lower limb rehabilitation	2-DOF: hip FE, knee FE	--	Kanno <i>et al.</i> [33]
		1-DOF: knee FE	Maximum load of up to 550 N	Macdaid <i>et al.</i> [34]

Lower orthotic gait training system (AIRGAIT)	Designed to regain the impaired movements for spinal cord injury patients	2-DOF: hip FE, knee FE	Maximum angle extension of up to 60° at knee joint	Dzahir <i>et al.</i> [38, 44, 45], Dao <i>et al.</i> [46, 47]
---	---	------------------------	--	---

FE = flexion/extension, AA = adduction/abduction, IE=inversion/eversion, DP=dorsiflexion/plantarflexion, UR=ulnar/radial deviation, SP = supination/pronation, LM=lateral-medial rotation, ROM=range of motion, ROT=range of torque, ROHM=range of human motion, ROHIS=range of human isometric strength

An overview on the mechanical design and assistance capacity of antagonistic-pair robots are demonstrated in TABLE I. It is noticed that PM antagonistic pairs have been widely adopted for almost all joints rehabilitation, especially for single-DOF joint. Since each antagonistic pair can only actuate 1-DOF motion, it is hard for them to guide and assist multi-DOF joints. Another limitation is that their assistance outputs are too small to cover the whole motion range of human joints. That means these robots may be just applicable to limited conditions and patients, instead of those who need larger assistance at the early stage of rehabilitation. To expand the assistance output, researchers have proposed several methods to modify the PMs antagonistic pairs, for example, doubling the numbers of PMs [36] and cooperating the mono-articular with bi-articular PM actuators [38, 44, 45].

B. Parallel Rehabilitation Robots

To achieve multi-DOF motion from one actuating joint, parallel PM configuration was proposed. Due to the high stiffness output and low inertia force, parallel configurations of PMs are mostly designed for ankle joint rehabilitation. University of Auckland developed a wearable 3-DOF ankle rehabilitation robot actuated by PMs in parallel, to correct the patient's gait pattern (Fig.2 (a)) [48]. The robot consists of two parallel platforms, a fixed platform and a moving platform that is actuated by four PMs in parallel [49]. As the PM can only provide unidirectional force, it is essential to add a redundant actuation to achieve the required motion DoFs. Since this orthosis enables patient's foot-ankle body fixed on the gaiter, the influence of knee joint's motion on the ankle can be mitigated. Likewise, the ankle rehabilitation robot proposed in [50] also employs parallel PMs to actuate the user's ankle joint (Fig.2 (b)). This orthosis allows the shinbone stay stationary during the ankle rehabilitation training. Southeast University, China, presented a humanoid lower limb exoskeleton (HLL) to assist knee and ankle joints motion [51]. However, not much details on the robot's performance were provided. Although parallel configuration is the mainstream structure for ankle rehabilitation, there are also some parallel PMs-driven rehabilitation robots for other multi-DOF joints. For example, Andrikopoulos *et al.* developed a 2-DOF PMs-actuated exoskeletal wrist (EXOWRIST) for wrist joint rehabilitation (Fig.2 (c)) [52, 53]. Four parallel PMs are placed on the plastic gloves around the forearm, to assist patients with the performance of main wrist activities. Since many patients have lost the controllability of their thumbs, they cannot perform main function of hands {Namazi, 2019 #36}. Shiota *et al.* presented a soft robotic rehabilitation system only for the thumb's movement ability reconstruction, as shown in Fig.2(d) [54]. In this design, parallel PMs placed on the forearm enable the thumb's metacarpophalangeal joint to achieve 3-DOF motion, and a soft pneumatic actuator for bending (SPAB) is used to assist the patient's thumb for bending motion.

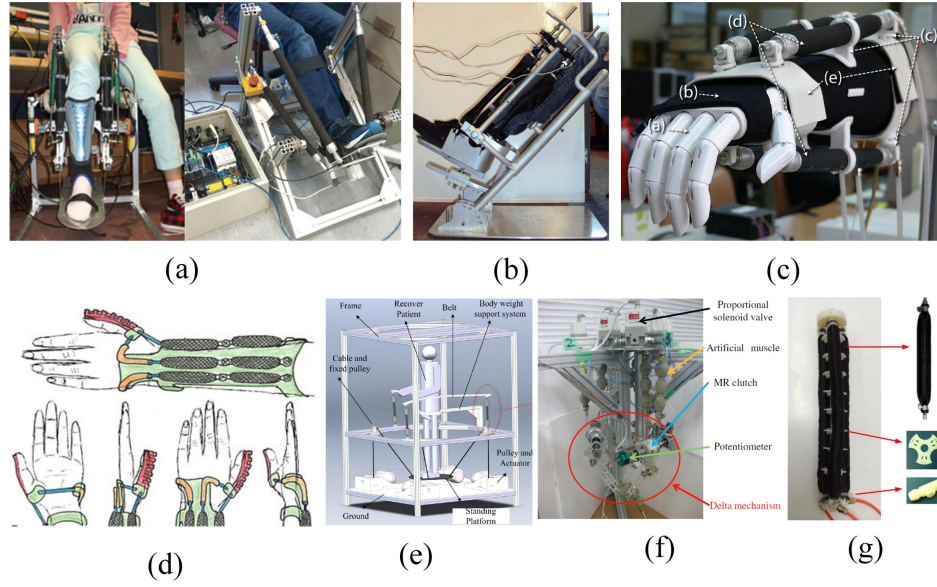


Fig.2. Antagonistic pair-type rehabilitation robots. (a, b) is reprinted from [49, 50], respectively; (c) is reprinted from [52], (d, e) is reprinted from [54, 55], respectively; (f) is reprinted from [14], (g) is reprinted from [56].

TABLE II
OVERVIEW OF PARALLEL REHABILITATION ROBOTS

Robots	Aims	Actuated DOFs	Assistance capacity	References
Wearable ankle robot	Providing the treatments of ankle sprain	3-DOF: ankle DP/IE/AA	100% of ROHM and ROT of 68~120 Nm	Jamwal <i>et al.</i> [48, 49]
Compliant ankle joint rehabilitation robot	Designed for home-based gait training associated with neurological disorders	3-DOF: ankle DP/IE/AA	--	Jamwal <i>et al.</i> [50]
Humanoid lower limb exoskeleton (HLLE)	Enhancing the power of person's lower limb	6-DOF: knee FE and ankle DP/IE	--	Wan <i>et al.</i> [51]
Exoskeletal wrist prototype (EXOWRIST)	Assisting wrist rehabilitation after stroke and sport injuries	2-DOF: wrist EF/UR	ROM of -41.7°~41.3°	Andrikopoulos <i>et al.</i> [52, 53]
Soft robotic thumb rehabilitation system	Providing rehabilitation for patients with thumb dyskinesia	4-DOF of thumb	100% of ROHM	Shiota <i>et al.</i> [54]
Hybrid-driven waist rehabilitation robot (HWRR)	Providing assistance for waist injured patients during rehabilitation training	Rotational 2-DOF	--	Zi <i>et al.</i> [55]
Delta-type parallel-link robot	Rendering human arbitrary-force sense for rehabilitation without force sensors	Translational 3-DOF	ROM of -50°~90°	Hirano <i>et al.</i> [14, 15]
Parallel actuator	A multi-DOF actuator for rehabilitation robots	Rotational 2-DOF and translational 1-DOF	The maximum strain is up to 40% of the actuator's initial length	Kang <i>et al.</i> [56]

FE = flexion/extension, AA = adduction/abduction, IE=inversion/eversion, DP=dorsiflexion/plantarflexion, UR=ulnar/radial deviation, SP = supination/pronation, LM=lateral-medial rotation, ROM=range of motion, ROT=range of torque, ROHM=range of human motion, ROHIS=range of human isometric strength

Aiming at the recovery for another multi-DOF joint, wrist, Zi *et al.* designed a hybrid-driven waist rehabilitation robot (HWRR) powered by three parallel PMs and springs (Fig.2(e)) [55]. Recently, the PMs-driven parallel configurations have attracted the widespread attentions. A straight-fiber-type PMs-actuated 3-DOF delta mechanism was developed by Chuo University, Japan (Fig.2 (f)) [14, 15]. The arms are actuated by parallel PMs through the pulley, and the end plate always remain parallel to the base plate, to achieve three translational DOFs. Its workspace is expanded, but the force output is still limited. To enable a fast response and high output, the team developed a modified version by adding magneto rheological (MR) clutches. Different from previous parallel configuration, Kang *et al.* designed a novel 3-DOF PM actuator with a compact and lightweight structure (Fig.2 (g)) [56]. The design consists of three PMs in parallel, and relative position of muscles is kept by eight connecting

plates. By regulating pressure in each PM, this actuator can provide one translational DOF and two rotational DOFs.

TABLE II shows the comparison of parallel PMs-driven rehabilitation robots. We can see that parallel configurations are suitable for multi-DOF joints rehabilitation, such as ankle, wrist and waist joints. But the number of relevant publications is exactly small, and some of them do not provide many details about the robots' assistance capacity. The mechanical complexity of parallel robots is greater than antagonistic pair-type ones, which may place a great obstacle on the parallel robot's applications in rehabilitation. Recently, several novel designs of parallel PMs-actuators have been published [14, 15, 56, 57], the adoption of these new parallel configurations may reduce the complexity of the rehabilitation robots. Additionally, the table demonstrates the larger output ability of parallel configurations, and they can cover the whole motion range of corresponding human joints. As these antagonistic and parallel configurations have their own special advantages and limitations, it may be a good choice to combine them together to develop multi-joint-multi-DOF rehabilitation robots.

C. Bio-Inspired Robots Design

To achieve more natural rehabilitation training, some researchers learnt from the human biological model and designed bio-inspired robots by actuating each PM independently, in which PMs imitate the working principle of human muscles. The soft ankle-foot orthotic device designed by Park *et al.* from Harvard University, US, is a typical example of bio-inspired PMs-actuated rehabilitation robots (Fig.3 (a)) [58, 59]. In this design, three PMs are attached on the anterior part of the lower leg, close to the biological tendons. The PMs work as actual anterior muscles for dorsiflexion independently. Moreover, this robot is mainly made of soft materials, without limitation of steel attachment, so it can help ankle joint to achieve 3-DOF motions in a large workspace. Recently, Alfahaam *et al.* proposed a wearable glove, employing four bending PMs to drive corresponding fingers respectively, as shown in Fig.3 (b) [60]. Experimental results show that the robot can assist most human hand activities. The team further developed a new wearable glove for wrist joint rehabilitation with a similar mechanical design [60] [61].

University of Michigan, US, designed a series of PMs-actuated ankle-foot orthosis, as presented in Fig.3 (d) [7, 62, 63]. They firstly designed two ankle-foot orthoses, one is a single-PM-actuated orthosis and the other is driven by two PMs in parallel. All these PMs are attached to the posterior of the orthoses, to provide plantarflexor torque [63]. The experimental results show that, the total force produced by two PMs is double of the force produced by a single PM. But there is no difference on the peak force. In the same year, the team proposed a modified ankle-foot orthosis (AFO) actuated by two PMs [7, 62]. One of the PMs is attached to the anterior to provide dorsiflexion torque, while the second one placed on posterior part to produce plantar flexion torque. The modified orthosis can provide patients with additional dorsiflexion motion assistance, but the torque outputs are too limited to satisfy the patients' gait rehabilitation. Afterwards, a knee-ankle-foot orthosis (KAFO) was developed to meet the rehabilitation demands for lower limbs [6]. In order to achieve larger torques to ensure the normal joint motion range, the orthosis is driven by six

PMs together via stainless steel brackets. Due to the trade-off between output torque and motion range of PMs, the knee torque is smaller than the ankle torque. Hence, combining other type of actuators with PMs is a good choice to improve the torque and motion abilities of the rehabilitation robots. For example, Hyon *et al.* designed a novel structure by combining PMs with electric motors (Fig.3 (c)) [64]. Attributing to the expanded motion range and output torque, the robot can help patients to squat and walk. In 2014, Adolf *et al.* proposed a robotic ankle orthotic device for patients with chronic ankle instability (CAI) (Fig.3 (e)) [65]. As shown in Fig.3(f), to make the device more wearable and light-weight, Irshaidat *et al.* proposed a soft arm exoskeleton (EpMAE) for patients performing repetitive motion therapy at home without the assist of therapists and with a lower cost [66]. Different from traditional mechanism design of supination and pronation, Zhang *et al.* designed a 2-DOF soft elbow rehabilitation exoskeleton with two PMs horizontally on both side of the beam while beams and the axis of joint are collinear. During the movement process, one actuator's compression enable the beam to twist and the other elongated one would help to release its pressure to beam turn back [67]. As shown in Fig.3(g), the PM actuators completely avoids the steel structure and can be wound around the patient's arm, which fits well with the human body but is difficult to wear. Deaconescu *et al.* developed a soft simultaneous passive rehabilitation robot for the the radiocarpal, metacarpophalangeal and interphalangeal joints of the hand (Fig.3(h).) [68].

In recent years, a series of upper limb rehabilitation robots (RUPERT) were developed by Arizona State University, US, as shown in Fig.3(i). RUPERT III, a 4-DOF therapeutic robot, is actuated by four PMs individually to assist shoulder extension, elbow extension, forearm supination/ pronation, and wrist extension [5, 69, 70]. This robot is back-drivable and safe for patients, but the gravity is not compensated and the motion range is limited. Therefore, shoulder external rotation has been added in RUPERT IV to expand the robot's workspace. Additionally, RUPERT IV is mainly made of graphite composite materials to reduce its weight, so that it can enhance the user's ability to perform activities of daily living [3, 4]. To stimulate patient's muscle activities and improve the robot-assisted performance, a hybrid robot assisted system powered by surface function electrical stimulation (FES) and PMs was developed [71].

As summarized in TABLE III, bio-inspired robots seem to be more mature than antagonistic and parallel robots, especially KAFO and RUPERT have been studied for years, perhaps attributing to their more simple and flexible design. Not limited to stiff support frame, the PMs even enable the fingers to perform some complex activities of human hands. From the view of theory, bio-inspired robots are supposed to cover the complete natural motion ranges for both human upper and lower limbs. But in practice, the current PM-driven robots cannot reach such a wide workspace due to the limitation of PM's output force. To expend the assistance capacity of the robots, other types of actuators have been used with PMs together to assist the patients [64].



Fig.3. Bio-inspired rehabilitation robots. (a-c) is reprinted from [58, 60, 64], respectively; (d) is reprinted from [6, 7, 62, 63], (e) is reprinted from [65], (f) is reprinted from [66], (g) is reprinted from [67], (h) is reprinted from [68], (i) is reprinted from [5, 69, 70].

TABLE III
OVERVIEW OF BIO-INSPIRED ROBOTS

Robotic system	Aims	Actuated DOFs	Assistance capacity	References
Soft ankle-foot orthotic device	Providing rehabilitate for patients with neuromuscular disorders	2-DOF: ankle DP/IE	ROM of 27° (14° dorsiflexion and 13° plantarflexion)	Park <i>et al.</i> [58, 59]
Wearable glove	Designed for power assistance rehabilitation for hands	Multi-finger FE	40%~45% of healthy person's force	Alfahaam <i>et al.</i> [60]
Wrist rehabilitation exoskeleton	Providing wrist joint rehabilitation	2-DOF: wrist FE/UR	ROM of 0~90° and 0~70° for FE; ROM of 0~50° and 0~20° for UR	Alfahaam <i>et al.</i> [61]
RUPERT III	Designed to assist patients with spasticity and hypertonia	4-DOF: shoulder/elbow/wrist extension, forearm supination	ROM of 15°~85°, 0~125°, 30°~60°, -45°~45°, respectively	Balasubramanian <i>et al.</i> [5, 69, 70]
RUPERT IV	Providing home-based and clinical therapies for stroke patients	5-DOF: add a shoulder external rotation based on RUPERT III 1-DOF: ankle DP	-- Maximum torque of 70Nm/38Nm, and ROM of 0~7°/0~15°	Balasubramanian <i>et al.</i> [3, 4] Ferris <i>et al.</i> [7, 62]
Soft arm exoskeleton (EpMAE)	Helping patients with repetitive motion therapy at home	1-DOF: elbow FE	Maximum angle of 0°~230°	Irshaidat <i>et al.</i> [66]
Soft elbow rehabilitation exoskeleton	Designed to assist the rehabilitation of elbow	2 DOF: elbow FE/ DP	Maximum angle of 0°~160° and 0°~90° for FE and DP respectively	Zhang <i>et al.</i> [67]

Soft simultaneous passive hand rehabilitation robot	Providing assistance for the the radiocarpal, metacarpophalangeal and interphalangeal joints	3-DOF: wrist FE, metacarpophalangeal joints FE	Maximum angle of 70°/ 80° for wrist FE, and 90°/ 100° for metacarpophalangeal joints FE	Deaconescu <i>et al.</i> [68].
Knee-ankle-foot orthosis (KAFO)	Assisting patients during walking	2-DOF: knee FE, ankle DP	22%~33% and 15%~33% of ROHIS for knee FE, and 42%~46% and 83%~129% of ROHIS for ankle DP	Sawicki <i>et al.</i> [6]
Hybrid drive exoskeleton robot (XoR)	Providing rehabilitation for the elderly, the strokes or people with spinal cord injury or stroke	10-DOF: hip FE/AA, knee FE, ankle FE/AA	Maximum angle of -120°/30°, -30°/30°, 0°/120°, -60°/30°, -30°/30°, respectively	Hyon <i>et al.</i> [64]
Lightweight compliant robotic ankle orthosis	Assisting gait treating for patients with chronic ankle instability (CAI)	2-DOF: ankle DP/IE	ROM of 28.4%~76% and walking range of 10%~72%	Adolf <i>et al.</i> [65]

FE = flexion/extension, AA = adduction/abduction, IE=inversion/eversion, DP=dorsiflexion/plantarflexion, UR=ulnar/radial deviation, SP = supination/pronation, LM=lateral-medial rotation, ROM=range of motion, ROT=range of torque, ROHM=range of human motion, ROHIS=range of human isometric strength

III. CONTROL STRATEGIES OF PMS-ACTUATED REHABILITATION ROBOTS

A. Control of Antagonistic Joints

In [22, 23, 38, 44, 72, 73], traditional PI and PID control were utilized to achieve the trajectory tracking for an upper limb exoskeleton and a walking assistive orthosis. But results from these papers show that, robustness and accuracy of PI/PID control strategies still need to be improved. Serious respond delay was found in some schemes, for example, there is 0.2 second delay for the 1 second gait circle in [44]. To adjust the robot assistance according to the human-robot interaction, Tsagarakis *et al.* introduced impedance control with torque feedback [23]. The results show that the output torque errors decrease from ± 2 Nm to ± 0.2 Nm. As the spasms of the stroke patient's muscle may cause abnormal events during the rehabilitation, force/position control is employed to enhance the training safety. Ahn *et al.* introduced neural networks to tune the gain parameters of PID controller, and compensate the disturbance [74, 75]. Then to improve the device's compliant output performance, they designed a new hybrid adaptive neural network compliant force/position controller (ADNN-PID) so that the 2-DOF robot's all nonlinear features can be dynamically identified [76]. Jiang *et al.* combined PID controller with position feedback to control antagonistic PM pairs [24]. The results show that there is no obvious trajectory tracking error, but existing an overshoot of about 1°. To reduce the overshoot, a neuron PI control approach was proposed by employing a neural network to tune the PI control gains [77]. Further, a feed-forward controller was utilized to relieve the system friction, which is main cause of the overshoot. Compared with traditional PI controller, overshoot of the proposed controller decreases from 6.35° to 2°. But it can only work well in a limited workspace. Likewise, researchers from Arizona State University utilized PID-based feedback control strategy for the RUPERT [4]. To ensure the maximum voluntary participation, an iterative learning controller was employed to determine and adjust the patient's reachable workspace.

Since FLC mainly depends on experiences instead of detailed and precise models, it is an effective scheme to deal with PMS-actuated robots. For example, Jiang *et al.* proposed a fuzzy neural network (FNN) controller for the 4-DOF upper limb exoskeleton [27]. Combined with neural network, FLC is reconstructed as a five-layer FNN controller. The parameters of the membership function layer and output layer are online updated through error back propagation training algorithm. Through

comparison with classical PI controller and FLC, FNN controller shows better performance with faster response and smaller vibration in trajectory tracking experiments. However, it is hard to obtain available experience-based data, and complicated fuzzy rule base usually increases the control complexity. To reduce the number of fuzzy rules, researchers proposed fuzzy sliding surface based on self-organizing learning mechanism (ASOFSMC) [78, 79]. Compared with the fuzzy sliding controller (ASMC), the steady-state error range of ASOFSMC decrease from 0.09~0.664 mm to 0.022~0.044 mm. Then the team employed functional approximation (FA) to update and adjust fuzzy parameters of the fuzzy sliding mode controller (ASTFC) [80]. The maximum motion error and phase lag of ASTFC decline by 42.86% and 37.5% than FSMC's, respectively. The experimental results validate the control system's excellent tracking performance to overcome external disturbance. For the power knee exoskeleton (KNEXO), Beyl *et al.* proposed a proxy-based sliding mode controller (PSMC), in which a virtual robot link was connected to the real link via a PID-type virtual coupling [16, 17]. This control scheme is designed to deal with the chattering problem of traditional SMC and make joints' motion smoother. Meanwhile, echo state network and nonlinear disturbance observer were also employed to compensate the control disturbance for the pneumatic muscle [81-83]. Likewise, a fuzzy logic controller was employed to approximate the switching control law [84], which can compensate the nonlinear disturbance effectively. In [85], Liu *et al.* proposed equivalent control-based discrete SMC (DSMC-EC) and exponential reaching law-based discrete SMC (DSMC-ER), with quicker response speed and smaller initial tracking error. Through introducing a feedforward torque by combining force sensor feedback with a feedforward element, the mean tracking error of the proposed control scheme decreases to 1.7°. As the PSMC approach lacks control robustness and adaptability, a neural network proxy-base sliding mode control (NNPSMC) strategy was presented in [37]. The gains of PSMC are tuned by neural network online, enhancing the adaptability to different conditions and patients. Hussain *et al.* proposed a boundary layer augmented sliding mode controller (BASMC) for trajectory tracking of hip and knee joints [42]. To promote the training safety, researchers employed joint compliance control to adjust the robot's output torque based on the human-robot impedance. Then the team developed assisted-as-needed gait training strategy by employing the adaptive impedance control approach [86]. Khajehsaeid *et al.* proposed an adaptive back stepping fast terminal sliding mode controller [87]. According to the individual's disability level and movement ability, the controller adjusts the robotic assistance to promote the human-robot interaction and patient's participation in rehabilitation training. As to the gait training robot AIRGAIT, the fractional order derivative was employed to modify the computed torque based on the mathematical model, which significantly improved in both transient and steady-state [88]. To enable the patients to be more active in their training, a new compliance controller was proposed to adjust the robot's assistance according to the human-robot interactive torque and human active torque. Finally, the effectiveness of the proposed strategy is confirmed by various experiments with the participation of eight healthy subjects. Particularly, all the subjects report that they feel comfortable during the experiments.

In previously mentioned approaches, the trajectory and compliance are all controlled by different single-input-single-output controllers, making it impossible to achieve complete synchronization between pressure and compliance. To address this problem, Cao *et al.* proposed a multi-input-multi-output controller, which can control the pressure and compliance at the same time [89]. However, the integral sliding surface of SMC accumulates the trajectory errors caused by structure uncertainties, making patients uncomfortable. To deal with the structure uncertainties, chattering-free robust variable structure control law (CRVC) and Proxy-based Sliding Mode Control were proposed in [90] and [91, 92]. The experimental results show that, the magnitude of angular deviations in the human-active training mode are 20° larger than passive training mode. Since better control compliance can promote patient's participation in the training, the angular deviations are acceptable.

TABLE IV
OVERVIEW OF CONTROL STRATEGIES FOR ANTAGONISTIC JOINT ROBOTS

Robotic system	Motion control strategy	Interactive control strategy	Validation	Performance	References
7-DOF upper limb exoskeleton	PID control	Impedance control with torque feedback	Trajectory tracking experiments and free motion experiments	The maximum motion error is less than 2.5%, and a fast response of 0.3 sec with an overshoot of 6%	Tsagarakis <i>et al.</i> [23]
Orthotic gait training system (AIRGAIT)	PI/PID controller	--	The basic function is tested by a healthy adult	The maximum angle error of 5° for the 1 second gait cycle	Dzahir <i>et al.</i> [38, 44]
Exoskeleton robotic arm	PD control	Force control/impedance control	Experiments of three tracking tasks	The torque decreased in less than 2 seconds if there is an instant spasm	Xiong <i>et al.</i> [72]
2-axes manipulator	Nonlinear PID control with neural network	--	Trajectory tracking experiments of sinusoidal waveforms	The motion bandwidth is less than 2 Hz	Ahn <i>et al.</i> [74-76]
Robotic arm	Position-position control	Force-force control	Trajectory tracking experiments of different control strategies	The response time to reach a peak torque is 1.3 sec, with a overshoot of about 1° .	Jiang <i>et al.</i> [24]
	Neuron PI control with feedforward control	--	Experiments of step response and position tracking for two position control schemes	The overshoot is less than 2°	Jiang <i>et al.</i> [77]
RUPERT	Adaptive PID-based feedback control	Iteration learning control	57 stroke patients went through a treatment	--	Huang <i>et al.</i> [4]
Upper limb rehabilitation robot	Fuzzy neural network (FNN) control	--	Comparison experiments of FNN controller with classical PI controller and fuzzy controller	The response time of FNN controller is fast more than 0.3 second than the other two controllers	Jiang <i>et al.</i> [27]
Rehabilitation robot	Adaptive self-organizing fuzzy sliding mode control (ASOFSMC)	--	Experiments of circle tracking tasks	The angel tracking error is less than 0.8°	Chang <i>et al.</i> [78, 79]
Soft rehabilitation machine	Adaptive self-tuning fuzzy control (ASTFC)	--	Experiments of single joint rehabilitation machine	The peak-peak error is 1% and phase lag is 0.1°	Chang <i>et al.</i> [80]
	Two-layer controller: RMFE and model based PID controller	--	The simulation of tracking a desired trajectory	The maximum angular deviation is less than 0.97°	Cao <i>et al.</i> [93]
Human-inspired exoskeleton (HuREx)	IFT-PID control with FF controller/ FB controller	Impedance control	Comparison experiments for different control strategy	The maximum position error less than 2° with some bumps	Kora <i>et al.</i> [94]
	SMC	Impedance control	The simulation and experiments for trajectory tracking with variable speed	It can achieve better tracking performance at walking frequency of 1.5 Hz than 0.25 Hz	Cao <i>et al.</i> [40]
Power knee exoskeleton (KNEXO)	Proxy-based sliding mode control (PSMC)	Force/torque control	Simulation	The mean tracking error is 1.7°	Beyl <i>et al.</i> [16, 17]
Treadmill-based gait training robotic orthosis	neural network proxy-base sliding mode control (NNPSMC)	--	Two healthy subjects participated in gait training	The trajectory errors are $\pm 2.5^\circ$ and $\pm 4^\circ$ for hip and knee joint, respectively	Huang <i>et al.</i> [37]
	Boundary layer augmented sliding mode control (BASMC)	Joint compliance control	Three healthy subjects (male/female, age 25-41 years) participated in experiments	The maximum trajectory tracking error is 10°	Hussain <i>et al.</i> [42]
Lower limb robotic orthosis	BASMC	Adaptive impedance control	Ten neurologically intact subjects were recruited to evaluate the system	The angular deviation is $3.96^\circ \pm 1.08^\circ$ and $14.22^\circ \pm 3.2^\circ$ in the inactive mode and active mode	Hussain <i>et al.</i> [86]
	CRVC	Adaptive	Ten neurologically intact	the trajectory-tracking errors of	Hussain <i>et al.</i>

	impedance control	subjects were recruited to evaluate the system	4.22° and 7.1° for hip and knee joints	<i>al.</i> [90]
	Multi-input-multi-output sliding mode control (MIMO SMC) for pressure and compliance	The experiments were conducted with five healthy subjects	The RMS error is of 2.11°~11.79° for the gait circle frequency of 0.2Hz~0.7Hz	Cao <i>et al.</i> [38, 44, 89, 91, 92]
AIRGAIT	Assisted-as-needed control	experiments with the participation of eight healthy subjects	The maximum comparative root mean square tracking error is less than 3°	Dao <i>et al.</i> [88]

As presented in TABLE IV, through adopting advanced motion control strategies, most of the robots has accomplished accurate trajectory tracking tasks. But overshoot and response delay seem to be common unsolved problems among these control schemes. The problems are mainly caused by PM's highly-nonlinear characteristics and hysteresis. Since the large overshoot will easily lead to a second harm to patients, the control robustness and stability are indispensable for rehabilitation robots. Model-based feedforward schemes have been adopted to tackle this problem [94]. Further, it can be found from Table IV that the limitation of PM's physical properties makes it hard to operate in high frequency. While this problem seems to exert trifling effect on rehabilitation performance, as most patients are unable to perform high-frequency training tasks. From the table, it is obvious that variable PID controllers are used widely in antagonistic joint robots, perhaps attributing to their simple structures and tuning rules. But these PID-based control strategies perform not well, usually with large tracking errors and overshoots. While SMC-based and FLC-based control schemes are confirmed greater robust and stable control ability than those based on PID. In the view of human-robot interaction, impedance control and force control are the most widely adopted schemes. However, nearly half of control systems in the table ignore the interactive control development. That means these robots lack the ability of adjusting the assistance output according to the human-robot interaction. Further, aiming at providing rehabilitation assistance for patients, the most significant indexes are patient's participation and sense of safety instead of motion accuracy. In this view, some control schemes' experimental results with a high motion error are acceptable, if they are capable of promoting the patient's participation. Additionally, among all these robots' validation experiments, less than 25% of the researches recruited human subjects to evaluate the robots' performance, and only one research team conducted the clinical testing with stroke patients [16, 17].

B. Control of Parallel Robots

For rehabilitation robots actuated by parallel PMs, through inverse kinematics and PM's model, the robot's trajectories are transformed to pressure inside PMs. To achieve the desired trajectory, parallel PMs must work simultaneously to produce appropriate torques and displacements at different speeds. Therefore, how to simultaneously control the multi-PMs in parallel is a challenge. Xie's team developed a simultaneous control approach for the ankle rehabilitation robot with four parallel PMs [49]. To achieve multi-PMs simultaneous control, an inverse kinematic model was introduced into the disturbance observer based FLC scheme. To further reduce the tracking errors caused by the PM's model uncertainties, a modified genetic algorithm (GA) was employed to optimize the parameters of FLC [48]. The experimental results show that the tracking error range decreased from -3~6 mm to -2~5 mm, which is 23.33% of maximum tracking error in [49]. Then a position-force feedback cascade controller was

proposed to enable the movement intention-directed trajectory adaptation and encourage human–robot engagement [95]. To solve the PM's nonlinear characteristics during operation and to tackle the human-robot uncertainties in rehabilitation at a 2-DOF parallel ankle rehabilitation robot, Ai et al. proposed a novel adaptive backstepping sliding mode control (ABS-SMC) method with an observer to estimate the human-robot external disturbance so that the controller adjust the robot output to accommodate external changes [96]. However these controllers largely depend on the PM's model, to entirely avoid influence of the model on control performance, recently the team proposed an iterative feedback tuning (IFT) control scheme [97]. As a model-free method, IFT control approach can automatically adjust robot-assistance through learning from the history data. Therefore the robot can help patients to perform better in the next rehabilitation period so as to promote their participation in training. The proposed method is confirmed an excellent learning capability for repeated rehabilitation training through experiments. For the ankle rehabilitation robot presented in [50], a boundary layer augmented sliding mode control (BASMC) approach presents a robust control ability through trajectory tracking experiments. To improve the rehabilitation performance, impedance control was employed to adjust the robot's compliance for patient's maximum voluntary participation [50]. Andrikopoulos et al. designed an advanced nonlinear PID (ANPID) control system for the wrist rehabilitation exoskeleton EXOWRIST, to strengthen the motion control adaptability [53]. Through adopting an auto-adjustable control gain based on error magnitude, the steady-state errors of ANPID controller decline by nearly 50% compared with the classical PID controller. While for the straight-fiber-type PMs-actuated delta robot, Hirano et al. developed an inverse dynamic model-based PI controller to control the PMs, introducing a feedback element to compensate the end position error [14, 15]. The experimental results show that steady-state error is less than 2mm. Based on the parallel structure's inverse kinematics and PM dynamic model, Kang et al. designed an inverse controller for a 3-DOF robot with three PMs in parallel [56]. Combined with position/force/vision feedback, the control system achieves the robust control of the robot.

TABLE V
OVERVIEW OF CONTROL STRATEGIES FOR PARALLEL ROBOTS

Robotic system	Motion control strategy	Interactive control strategy	Validation	Performance	References
Wearable ankle rehabilitation robot	Adaptive FLC with fuzzy-based disturbance observer (FBDO)	--	A healthy subject (male, age 25 years) participated in the study	Maximum tracking error is ± 15 mm, and the MSE is 0m	Jamwal <i>et al.</i> [48]
	Modified genetic algorithm (GA) based fuzzy feedback control	--		Maximum tracking errors are -2~5mm	Jamwal <i>et al.</i> [49]
	position-force feedback cascade controller	Force feedback control	A healthy subjects participated in experiments	The maximum tracking error are all less than 2.3%	Zhang <i>et al.</i> [95].
	Robust iterative feedback tuning (IFT) control	--	Motion performances are evaluated by four participants	Peak amplitude errors are less than 2°	Meng <i>et al.</i> [97]
Compliant ankle rehabilitation robot	adaptive backstepping sliding mode control (ABS-SMC)	--	Five healthy subjects participated in experiments	The maximum tracking error with the interaction with subjects is 7.5 mm	Ai <i>et al.</i> [96]
	Boundary layer augmented sliding mode control (BASMC)	Impedance control	Ten healthy subjects participated in experiments	The maximum angular deviation is 0.252 rad	Jamwal <i>et al.</i> [50]
Exoskeletal wrist prototype (EXOWRIST)	Advanced nonlinear PID (ANPID) control	--	A healthy subject is recruited to evaluate the device's motion capabilities	The mean absolute steady-state errors of 0.22° ~0.41°	Andrikopoulos <i>et al.</i> [53]
Delta-type	Feedback PI control	--	Position-control and	The average errors are	Hirano <i>et al.</i> [14,

parallel-link robot			stiff-control experiments	1.25~3.53 mm on each axis	15]
Parallel actuator	Inverse control	Force/vision feedback control	Simulations and experiments of extension and bending motion	The accuracy is approximately 2% of the initial length	Kang <i>et al.</i> [56]

TABLE V demonstrates the control strategies and their performances. Only fewer than half of the robotic systems in the table own an adaptability towards the patient's disability and motion level. Modified genetic algorithm and iterative feedback tuning schemes are popular approaches to strengthen the control adaptability. Although most of the research teams have conducted validation experiments with human subjects, none of them evaluated their robot's rehabilitation performance through clinical measurements. From the view of motion control, all of these robotic rehabilitation systems have achieved high accuracy and stability in trajectory tracking experiments. In addition, among these control schemes, half of them increase the robustness and accuracy through tuning the control parameters by position/force feedback.

C. Control of Other Robots

It has been found that an obvious correlation exists between electromyography signals, limb movements and muscle activities. EMG-based control strategies have been widely used in PMs-driven rehabilitation robots. Researchers from Harvard University proposed a proportional EMG control approach to control the corresponding muscles for ankle rehabilitation [58]. However, the results show that joint motion range, safety and stability of the approach remain to be improved. To address this problem, the team proposed a linear time-invariant (LTI) controller [59]. Through adopting the subspace system identification technique avoids complex modelling of human-robot system. However the experimental results show that, the tracking error will rise if the frequency and tracking angle increase. Likewise, a similar scheme was utilized to control a glove actuated by four bending muscles, to achieve the hand's pinch and grip movement [60]. For the soft arm exoskeleton for patients performing repetitive motion therapy at home, a Model Reference Adaptive Control (MRAC) has been proposed for adhering to target rehabilitation profiles [66]. For the PMs-actuated ankle-foot orthosis, based on proportional EMG (PM) control approach, artificial dorsiflexor and flexor are regulated by biological tibialis anterior and soleus respectively [7, 62]. To relieve co-activation between the artificial flexor and dorsiflexor, the researchers combined flexor inhibition with proportional EMG control (PMFI), and the peak powers grow by nearly 30% over PM control [6]. The main unsolved problem for controlling bio-inspired rehabilitation robots is to obtain effective EMG signals. At present, it is extremely hard to obtain the complete same EMG signals from different person for the same motion, even from the same person. For RUPERT, researchers just adopted an open loop feedforward control to achieve arm reaching tasks [5]. The results show that the control scheme exists a large steady state error when the patient lacks control ability. To tackle this problem, a PID feedback controller was adopted to guide each joint's motion [3]. While there is a response delay for the robot to reach the desired angle, about 3 seconds. To compensate the PM's slow response, iterative learning control (ILC)-based feedforward controller was introduced [4]. Through learning from errors in previous executions, ILC optimizes the control

parameters and thus improves the control performance. Then fifty-five patients were recruited to participated in the clinical testing, and the mean Fugl-Meyer score of those subjects grew from 97 to 103.5.

From TABLE VI, bio-inspired habilitation robots are mainly controlled by proportional EMG control approaches. Through directly controlling the PMs by EMG signal, the robots are capable of assisting patients in a more natural way. But the majority of the current control systems still focus on the basic proportional EMG control approaches, the trajectory tracking errors are usually quite large, as shown in the table. For RUPERT, researchers recruited patients to participate the clinical testing and their robot-assisted rehabilitation performance are evaluated by professional assessment standards. Irshaidat *et al.* proposed a soft arm exoskeleton for patients performing repetitive motion therapy at home without the assist of therapists and with a lower cost [66].

TABLE VI
OVERVIEW OF CONTROL STRATEGIES FOR OTHER ROBOTS

Robotic system	Motion control strategy	Interactive control strategy	Validation	Performance	References
Soft ankle-foot orthotic device	Feedback proportional EMG control		Validation experiments of mechanical characterization and control function	The capability of disturbance rejection capacity is 5°	Park <i>et al.</i> [58]
	Linear time-invariant (LTI) control		The suitability validation with six sets of different experiments	The mean tracking error range is 7.4%~20.2% for frequency of 0.4 Hz~1.0 Hz with angle of 10°	Park <i>et al.</i> [59]
Wearable glove	Feedback proportional EMG control		Healthy males and females (age over 50) participated in experiments	The EMG signals with the glove is about 25% of which without the glove	Alfahaam <i>et al.</i> [60]
Arm exoskeleton	Model Reference Adaptive Control		Position control	It can vary from 0° to 180° ideally	Irshaidat <i>et al.</i> [66]
Ankle-foot orthosis (AFO)	Proportional soleus EMG control		A healthy subject (age 30 years) test the device's performance	It can provide 36% and 123% of the peak torque for plantar flexor and dorsiflexor, respectively	Ferris <i>et al.</i> [7, 62]
Knee-ankle-foot orthosis (KAFO)	Proportional EMG control with flexor inhibition		Three healthy male subjects participated in the study	It can provide 42% and 83% of peak power for plantar flexor and dorsiflexor, respectively	Sawicki <i>et al.</i> [6]
RUPERT series of robots	Open loop feedforward control	--	Ten patients went through the clinic testing	The device can expand motion workspace of about 50° for subject's shoulder/elbow/wrist, respectively	Sugar <i>et al.</i> [5]
	PID-based feedback control	Iterative learning control based feedforward control	57 stroke patients went through the treatment	The mean Fugl-Meyer score increases by 6.5 through treatment	Balasubramanian <i>et al.</i> [3]

Compared with traditional rigid actuators, PMs are more compliant and safer, which plays a vital role on the patient's rehabilitation, but their highly nonlinear and time-varying properties arise difficulties in precise control of PMs-actuated robots. PID control, fuzzy logic control (FLC), and sliding model control (SMC) are widely adopted control approaches, attributing to their ability to develop a simple and robust control system. Actually, the choice of different control strategies usually depends on the structure of PMs-actuated robots and movement requirements. Recently, in order to ensure the patient's maximum voluntary participation, researchers started to conduct research on interactive control strategies, adjusting the assistance output according to the patient's disability level, rehabilitation stage and motion intention [98]. However, it is hard to utilize the former two control strategies in complexed and nonlinear PMs-driven robots, due to their linear control structure or too overly complicated rules [99]. To tackle these problems, Ziegler-Nichols [100], inverse NARX fuzzy model [101], and other knowledge-based adaptive compensator [102] were employed to enhance the performance of PID control and fuzzy control [103]. Compared with PID, sliding

mode controller (SMC) can switch between various control structures to adapt to the current state and is able to compensate PM's unpredicted disturbances and model uncertainties. However, due to high switching frequency, the chattering problem always exists. To tackle the problem, Xing *et al.* introduced a nonlinear disturbance observer to reduce the switch gain of SMC system [104]. Likewise, a fuzzy logic controller was employed to approximate the switching control law [105], which can compensate the nonlinear disturbance effectively. For the ankle rehabilitation robot driven by PMs in parallel configuration, the control difficulties not only relate to PM's highly nonlinear and time-varying characteristics, but also caused by coupling interference from multiple PMs' synchronous movement. However, few studies focused on the collaborative control between multiple PMs and the disturbance elimination. Although Cao *et al.* proposed a multi-input multi-output controller, which is designed to control the pressure and compliance for a single PM at the same time, instead of synchronizing the movement of multiple PMs [89].

IV. DISCUSSION

Attributing to the inherent compliance and safety, PMs are exactly appropriate to actuate rehabilitation robots. Although most of the existing PMs-actuated rehabilitation robots have shown their assistance capacity, many common unsolved problems remain. As a bio-inspired actuator, the respond speed and accuracy of current PMs still need to be improved to simulate biological muscles. Recently, several innovative PMs were designed, such as straight-fiber-type muscles [14, 15], pleated pneumatic artificial muscles [16, 17], and spring over muscles [106]. Although many PMs-driven exoskeletons are claimed as wearable rehabilitation robots, most of them cannot achieve several-hour's training with the limitation of energies. With heavy weight, large occupied space, power source in previous researches arise the difficulties in practical applications for clinical treatments and patient's rehabilitation training at home. Hence it is obliged to develop wearable and cost-effective gas supply approaches, for example, a solid storage of hydrogen gas has been studied in [107, 108]. Additionally, for wearable rehabilitation robots, especially upper limb exoskeleton, the heavy weight and complex mechanism of the devices cause external burden for patients and arise control difficulties. Recent researches employed advanced materials and manufacturing technology to make robots more lightweight and strengthen the output assistance, for example, using advanced soft elastic driving material [109, 110], carbon fibers [111], hybrid-driven technology [112-115] and 3D printed materials [34, 40, 116]. Moreover the compliance and morphology of wearable robots preclude the use of many conventional sensors including encoders, metal or semi-conductor strain gauges, or inertial measurement units. To further achieve the potential of a wearable robotic system in different rehabilitation training conditions, the sensing devices are expected to be embedded in the PMs-driven flexible-bending structure, soft & smart materials and stretchable electronics [19]. Since the sensing system in wearable human-robot rehabilitation application cannot increase the burden on the patients, an advanced sensing device is supposed to own the capability of monitoring multiple physical or physiological signals at the same time. Thus some promising measurement technology, such as technology of fiber Bragg gratings, have attracted a wide spread attention. With the

layered structures, it is possible for these sensors to simultaneously measure displacement [117], motion speed [21], joint angle [22], plantar pressure [23], interaction force [24], muscular tension [25], and so on. The maximum assistance output produced by the existing rehabilitation robots are limited, most of them even cannot cover the complete human natural workspace. This drawback may not exert obvious effect when patients are at early rehabilitation stage, but it precludes robots from providing further function recovery for patients after several training sessions. To address this problem, it is good to combine other type actuators or muscle-stimulating technologies with PMs, e.g., electric motors [64] and functional electrical stimulation (FES) [43, 118] have been studied recently. In the view of humanized design, studies on the biological musculoskeletal system among patients and healthy person will deepen the understanding of patient's rehabilitation needs. Furthermore, it also helps researchers to take full advantages of the PM's bio-mimetic functionality and medical applicability, to develop more practical and humanized rehabilitation robot for each individual patient.

In terms of control strategies of rehabilitation robots, PM's highly-nonlinear, time-varying and delay response properties arise difficulties in PMs-actuated rehabilitation robots control. The neglected or un-modelled elements of PM's dynamic models introduce uncertainty and disturbance for control system. Some recent studies have considered PM's un-modelled elements, for example, dynamic models with hysteresis element were proposed in [21]. In aspect of improving the control adaptability, the cooperation between the advanced control strategies and sensing-fusion may make sense, such as mechanical sensing [119] and bio-sensing [120]. As the state-of-the-art sensors can not only monitor the patient's real-time motion, but also catch his/her small reaction changes, the robots are capable of adjusting the control scheme on time, enhancing the control robustness and adaptability. For example, a light-weight PMs-driven walking assist system according to the patient's lower limb force on-line feedback has been proved its effectiveness for reducing knee joint force during walking [121]. To make patients feel safe and comfortable during training, the robot's compliance should be adjusted according to the human-robotic interaction. Some researches even considered the instant spasms of stroke patients [23]. To promote the patient's voluntary participation, advanced assist-as-needed interactive control strategy is an indispensable factor in the future. In this way, patients are allowed to stimulate and regulate the robotic assistance according to their motion intention, and they will be encouraged to participate in rehabilitation training. And the far-reaching effect of human-robot interaction on rehabilitation performance have been confirmed by large number of researches, especially motor imagery-based brain computer interface [10, 122, 123]. Additionally, integrating the robot-assistance with vision feedback [9, 122] and visual reality [11, 125, 126] will further enhance patient's voluntary participation in the training process. In the future, the intelligent control strategies and personalized training modes will be developed, making robots adaptable to various patients according to their disability levels, recovery stage, physical conditions, age difference and rehabilitation demands. The control strategies and training modes will be expected to be conducted under the guidance of medical standards [11] and professional therapists [126]. Consequently, the patients can receive professional and effective rehabilitation assistance.

Finally, most current researchers conducted trajectory tracking experiments to confirm the function of the robotic system, but just few of them carried out clinical testing validation for robot-assisted rehabilitation training [11, 127, 128]. Only through long training term clinical trials with a large scale of patients, the performance of rehabilitation robot system can be validated and optimized efficiently. Furthermore, the patient's rehabilitation performance needs to be evaluated by the professional rehabilitation assessment standards, such as Fugl–Meyer assessment [11], quality of life [129,130], and the patient's global impression of change [131] and the universal assessment standards [132]. Recently, the universal assessment standards has been established among rehabilitation engineering, clinical medicine and robotic engineering [132,133]. The professional clinical assessment will further help the researchers understand the patient's demands and robot's limitations, and find out the correct direction of improvement.

V. CONCLUSION

This paper conducts a review on mechanical structures and control strategies of PMs-actuated rehabilitation robots. Various PMs-actuated rehabilitation robots with diverse structures are discussed and compared, and the configuration characteristics are described. The information of existing advanced robot structures presented in this paper will provide inspiration and valuable knowledge for future rehabilitation robot development. Considering PM's nonlinear and time-varying prosperities, as well as variable PM-actuated structures, this paper presents well-established motion control schemes. To further promote the patient's training participation and rehabilitation performance, interactive control strategies are also highlighted. This paper is expected to be reliable guidance and comprehensive resources for researchers in the PM-actuated rehabilitation robot field.

REFERENCES

- [1] [Online]. Available: <http://www.world-heart-federation.org/cardiovascular-health/stroke/>.
- [2] [Online]. Available: http://www.cdc.gov/dhdspl/data_statistics/fact_sheets/fs_stroke/.
- [3] Balasubramanian S, Wei R, Perez M, and Shepard B, "RUPERT: An exoskeleton robot for assisting rehabilitation of arm functions," in *Virt Rehab*, Vancouver, BC, Canada, 2008, p. 163-167.
- [4] Huang J, Tu X, and He J, "Design and evaluation of the RUPERT wearable upper extremity exoskeleton robot for clinical and in-home therapies," *IEEE T Syst Man Cybern Syst*, vol. 46, pp. 926-935, 2016.
- [5] Sugar TG, He J, Koeneman EJ, and Koeneman JB, "Design and control of RUPERT: A device for robotic upper extremity repetitive therapy," *IEEE T Neural Syst Rehab Eng*, vol. 15, pp. 336-346, 2007.
- [6] Sawicki GS and Ferris DP, "A pneumatically powered knee-ankle-foot orthosis (KAFO) with myoelectric activation and inhibition," *J Neuroeng Rehab*, vol. 6, pp. 23-39, 2009.
- [7] Ferris DP, Czerniecki JM, Hannaford B, Michigan UO, Washington UO, and System VPSH, "An ankle-foot orthosis powered by artificial pneumatic muscles," *J Appl Biomech*, vol. 21, pp. 189-197, 2005.
- [8] Knaepen K, Mierau A, Swinnen E, Tellez HF, Michielsen M, Kerckhofs E, *et al.*, "Human-robot interaction: does robotic guidance force affect gait-related brain dynamics during robot-assisted treadmill walking?," *Plos One*, vol. 10, p. e0140626, 2015.
- [9] Wagner J, Solisescalante T, Scherer R, Neuper C, and Müllerputz G, "It's how you get there: walking down a virtual alley activates premotor and parietal areas," *Frontiers in human neuroscience*, vol. 8, p. 93, 2014.
- [10] Brauchle D, Vukelić M, Bauer R, and Gharabaghi A, "Brain state-dependent robotic reaching movement with a multi-joint arm exoskeleton: combining brain-machine interfacing and robotic rehabilitation," *Frontiers in human neuroscience*, vol. 9, p. 564, 2014.

- [11] Klamroth-Marganska V, Blanco J, Campen K, Curt A, Dietz V, Ettl T, *et al.*, "Three-dimensional, task-specific robot therapy of the arm after stroke: a multicentre, parallel-group randomised trial," *Lancet Neurology*, vol. 13, p. 159, 2014.
- [12] Tondu B, Ippolito S, Guiochet J, and Daidie A, "A seven-degrees-of-freedom robot-arm driven by pneumatic artificial muscles for humanoid robots," *Int J Robot Res*, vol. 24, pp. 257-274, 2005.
- [13] Saikawa T, "Development of a pneumatic artificial muscle based on biomechanical characteristics," in *IEEE Int. Conf Ind Technol*, Maribor, Slovenia, Slovenia, 2004, p. 729-734.
- [14] Hirano J, Tanaka D, Watanabe T, and Nakamura T, "Development of delta robot driven by pneumatic artificial muscles," in *IEEE/ASME Int Conf AIM*, Besancon, France, 2014, p. 1400-1405.
- [15] Kobayashi M, Hirano J, and Nakamura T, "Development of delta-type parallel-link robot using pneumatic artificial muscles and MR clutches for force feedback device," in *Int Conf Intell Rob Appl*, Portsmouth, UK, 2015, p. 410-420.
- [16] Beyl P, Van Damme M, Van Ham R, Vanderborght B, and Lefeber D, "Design and control of a lower limb exoskeleton for robot-assisted gait training," *Appl Bionics Biomech*, vol. 6, pp. 229-243, 2009.
- [17] Beyl P, Knaepen K, Duerinck S, Damme MV, Vanderborght B, Meeusen R, *et al.*, "Safe and compliant guidance by a powered knee exoskeleton for robot-assisted rehabilitation of gait," *Adv Robotics*, vol. 25, pp. 513-535, 2011.
- [18] An S, Kang DJ, and Yarin A, "Blister-like Soft Nano-textured Thermo-pneumatic Actuator as an Artificial Muscle," *Nanoscale*, 2018.
- [19] Zhao L, Cheng H, Xia Y, and Liu B, "Angle tracking adaptive backstepping control for a mechanism of pneumatic muscle actuators via an AESO," *IEEE T Ind Electron*, vol. PP, pp. 1-1, 2018.
- [20] Peng ZQ and Huang J, "Soft Rehabilitation and Nursing-Care Robots: A Review and Future Outlook," *Applied Sciences-Basel*, vol. 9, Aug 2019.
- [21] Yao BT, Zhou ZD, Liu Q, and Ai QS, "Empirical modeling and position control of single pneumatic artificial muscle," *J Control Eng Appl Inf*, vol. 18, pp. 86-94, Jun 2016.
- [22] Caldwell DG and Tsagarakis N, "Biomimetic actuators in prosthetic and rehabilitation applications," *Technol Health Care*, vol. 10, pp. 107-120, 2002.
- [23] Tsagarakis NG and Caldwell DG, "Development and control of a 'soft-actuated' exoskeleton for use in physiotherapy and training," *Auton Robot*, vol. 15, pp. 21-33, 2003.
- [24] Jiang X, Xiong C, Sun R, and Xiong Y, "Characteristics of the robotic arm of a 9-DoF upper limb rehabilitation robot powered by pneumatic muscles," in *Int Conf Intell Rob Appl*, Berlin, Heidelberg, Germany, 2010, p. 463-474.
- [25] Chen W, Xiong C, Xun R, and Huang X, "A 10-degree of freedom exoskeleton rehabilitation robot with ergonomic shoulder actuation mechanism," *Int J Hum Rob*, vol. 08, pp. 47-71, 2011.
- [26] Xing K, Huang J, Wang Y, He J, Xu Q, and Wu J, "Sliding mode tracking for actuators comprising pneumatic muscle and torsion spring," in *Int Conf Rob Biomim*, Guilin, China, 2009, p. 420-425.
- [27] Jiang X, Wang Z, Zhang C, and Yang L, "Fuzzy neural network control of the rehabilitation robotic arm driven by pneumatic muscles," *Ind Robot*, vol. 42, pp. 36-43, 2015.
- [28] Tang Z, Zhang K, Sun S, Gao Z, Zhang L, and Yang Z, "An upper-limb power-assist exoskeleton using proportional myoelectric control," *Sensors*, vol. 14, pp. 6677-6694, 2014.
- [29] Guo XX, Liu Q, Zuo J, Meng W, Ai QS, Zhou ZD, *et al.*, "A Novel Pneumatic Artificial Muscle -driven Robot for Multi-joint Progressive Rehabilitation," in *2018 Joint Ieee 8th International Conference on Development and Learning and Epigenetic Robotics*, ed, 2018, p. 78-83.
- [30] Meng W, Sheng B, Klinger M, Liu Q, Zhou Z, and Xie SQ, "Design and control of a robotic wrist orthosis for joint rehabilitation," in *IEEE Int Conf AIM*, Busan, South Korea, 2015, p. 1235-1240.
- [31] Noda T, Teramae T, Furukawa J, Ogura M, Okuyama K, Kawakami M, *et al.*, "Development of Shoulder Exoskeleton toward BMI triggered Rehabilitation Robot Therapy," in *2018 Ieee International Conference on Systems, Man, and Cybernetics*, ed, 2018, p. 1105-1109.
- [32] Caldwell DG, Tsagarakis NG, Kousidou S, Costa N, and Sarakoglou L, ""Soft" exoskeletons for upper and lower body rehabilitation - design, control and testing," *Int J Hum Rob*, vol. 4, pp. 549-573, 2007.
- [33] Kanno T, Morisaki D, Miyazaki R, Endo G, and Kawashima K, "A walking assistive device with intention detection using back-driven pneumatic artificial muscles," in *IEEE Int Conf Rehab Rob*, Singapore, Singapore, 2015, p. 565-570.
- [34] Mcdaid A, Kora K, Xie S, Lutz J, and Battley M, "Human-inspired robotic exoskeleton (HuREx) for lower limb rehabilitation," in *IEEE Int Conf Mech Autom*, Takamatsu, Japan, 2013, p. 19-24.
- [35] Hussain S, Xie SQ, Jamwal PK, and Parsons J, "An intrinsically compliant robotic orthosis for treadmill training," *Med Eng Phys*, vol. 34, pp. 1448-1453, 2012.
- [36] Cao J, Xie SQ, McDaaid A, and Das R, "Sliding mode control of an exoskeleton gait rehabilitation robot driven by pneumatic muscle actuators," in *IEEE/ASME Int Conf Mech Embed Syst Appl*, Boston, Massachusetts, USA, 2015, p. V009T07A002-V009T07A002.
- [37] Huang M, Huang X, Tu X, Li Z, and Wen Y, "An online gain tuning proxy-based sliding mode control using neural network for a gait training robotic orthosis," *Clus Comput*, pp. 1-14, 2016.
- [38] Mat Dzahir MA, Nobutomo T, and Yamamoto SI, "Development of body weight support gait training system using pneumatic Mckibben actuators -control of lower extremity orthosis," *Int Conf IEEE EMBC*, vol. 2013, pp. 6417-6420, 2013.

- [39] Huo W, Mohammed S, Moreno JC, and Amirat Y, "Lower limb wearable robots for assistance and rehabilitation: A state of the art," *IEEE Syst J*, vol. 10, pp. 1-14, 2014.
- [40] Cao J, Mcdaid A, Kora K, and Xie S, "Control strategies for human-inspired robotic exoskeleton (HuREx) gait trainer," in *IEEE/ASME Int Conf Mech Embed Syst Appl*, Auckland, New Zealand, 2016, p. 1-6.
- [41] Hussain S, Xie SQ, and Jamwal PK, "Robust nonlinear control of an intrinsically compliant robotic gait training orthosis," *IEEE T Syst Man Cybern Syst*, vol. 43, pp. 655-665, 2013.
- [42] Hussain S, Xie SQ, and Jamwal PK, "Control of a robotic orthosis for gait rehabilitation," *Robot Auton Syst*, vol. 61, pp. 911-919, 2013.
- [43] Tu XK, Huang J, He JP, and Ieee, "Leg hybrid rehabilitation based on hip-knee exoskeleton and ankle motion induced by FES," in *IEEE/ICARM Int Conf Adv Rob Mech*, Macau, China, 2016, p. 237-242.
- [44] Dzahir MAM, Nobutomo T, and Yamamoto SI, "Antagonistic mono- and bi-articular pneumatic muscle actuator control for gait training system using contraction model," in *Biosig Biorob Conf*, Rio de Janeiro, Brazil, 2013, p. 1-6.
- [45] Mat Dzahir MA, Nobutomo T, and Yamamoto SI, "Development of Gait Training System Powered by Antagonistic Mono-and Bi-Articular Actuators Using Contraction Model Control Scheme," *Appl Mech Mater*, vol. 393, pp. 525-531, 2013.
- [46] Dao QT and Yamamoto S, "Adaptive Impedance Control of a Robotic Orthosis Actuated by Pneumatic Artificial Muscle," in *World Congress on Medical Physics and Biomedical Engineering 2018, Vol 2*. vol. 68, L. Lhotska, L. Sukupova, I. Lackovic, and G. S. Ibbott, Eds., ed, 2019, p. 631-636.
- [47] Dao QT, Nguyen ML, and Yamamoto S, "Discrete-Time Fractional Order Integral Sliding Mode Control of an Antagonistic Actuator Driven by Pneumatic Artificial Muscles," *Applied Sciences-Basel*, vol. 9, Jun 2019.
- [48] Xie SQ and Jamwal PK, "An iterative fuzzy controller for pneumatic muscle driven rehabilitation robot," *Expert Syst Appl*, vol. 38, pp. 8128-8137, 2011.
- [49] Jamwal PK, Xie SQ, Hussain S, and Parsons JG, "An adaptive wearable parallel robot for the treatment of ankle injuries," *IEEE/ASME Trans Mech*, vol. 19, pp. 64-75, 2014.
- [50] Jamwal PK, Hussain S, Ghayesh MH, and Rogozina SV, "Impedance control of an intrinsically compliant parallel ankle rehabilitation robot," *IEEE T Ind Electron*, vol. 63, pp. 3638-3647, 2016.
- [51] Wan S, Yang M, Xi R, Wang X, Qian R, and Wu Q, "Design and control strategy of humanoid lower limb exoskeleton driven by pneumatic artificial muscles," in *Int Conf M2VIP*, Nanjing, China, 2016, p. 1-5.
- [52] Andrikopoulos G, Nikolakopoulos G, and Manesis S, "Design and development of an exoskeletal wrist prototype via pneumatic artificial muscles," *Meccanica*, vol. 50, pp. 2709-2730, 2015.
- [53] Andrikopoulos G, Nikolakopoulos G, and Manesis S, "Motion control of a novel robotic wrist exoskeleton via pneumatic muscle actuators," in *Emerg Tech Fact Autom*, 2015, p. 1-8.
- [54] Shiota K, Tarvainen TV, Sekine M, Kita K, and Yu W, "Development of a robotic thumb rehabilitation system using a soft pneumatic actuator and a pneumatic artificial muscles-based parallel link mechanism," in *Int Conf Intell Auton Syst*, 2016, p. 525-537.
- [55] Zi B, Yin G, and Zhang D, "Design and Optimization of a Hybrid-Driven Waist Rehabilitation Robot," *Sensors (Basel)*, vol. 16, Dec 14 2016.
- [56] Kang R, Guo Y, Cheng K, and Chen L, "Design and control of a soft actuator driven by pneumatic muscles," in *Int Conf Ind Autom Inf Commun Tech*, Bali, Indonesia, 2014, p. 26-30.
- [57] Zang WS, Zang KJ, Shen G, Li X, and Li G, "Position, Jacobian, decoupling and workspace analysis of a novel parallel manipulator with four pneumatic artificial muscles," *Journal of the Brazilian Society of Mechanical Sciences and Engineering*, vol. 41, Mar 2019.
- [58] Park YL, Chen BR, Young D, and Stirling L, "Bio-inspired active soft orthotic device for ankle foot pathologies," in *IEEE/RSJ Int Conf Intell Rob Syst*, San Francisco, CA, USA, 2011, p. 4488-4495.
- [59] Park Y, Chen B, Perez Arancibia, Young D, Stirling L, Wood RJ, *et al.*, "Design and control of a bio-inspired soft wearable robotic device for ankle-foot rehabilitation," *Bioinspir Biomim*, vol. 9, Mar 2014.
- [60] AlFahaam H, Davis S, and NeftiMeziani S, "Power assistive and rehabilitation wearable robot based on pneumatic soft actuators," in *Int Conf MMAR*, Miedzydroje, Poland, 2016, p. 472-477.
- [61] Al-Fahaam H, Davis S, and Nefti-Meziani S, "Wrist rehabilitation exoskeleton robot based on pneumatic soft actuators," in *ISCAE*, Newcastle upon Tyne, UK, 2016, p. 491-496.
- [62] Ferris DP, Gordon KE, Sawicki GS, and Peethambaran A, "An improved powered ankle-foot orthosis using proportional myoelectric control," *Gait Posture*, vol. 23, p. 425, 2006.
- [63] Gordon KE, Sawicki GS, and Ferris DP, "Mechanical performance of artificial pneumatic muscles to power an ankle-foot orthosis," *J Biomech*, vol. 39, pp. 1832-1841, 2006.
- [64] Hyon S, Morimoto J, Matsubara T, and Noda T, "XoR: Hybrid drive exoskeleton robot that can balance," in *IEEE/RSJ Int Conf Intell Rob Syst*, San Francisco, CA, USA, 2011, p. 3975-3981.
- [65] Adolf G, Bolton M, Bonia T, Daly S, Maurice O, Murphy P, *et al.*, "Development of A Robotic Device to Improve Chronic Ankle Instability through Controlled Perturbation," in *Annual Northeast Bioeng Conf*, Boston, MA, USA, 2014.
- [66] Irshaidat M, Soufian M, Al-Ibadi A, Nefti-Meziani S, and Ieee, *A Novel Elbow Pneumatic Muscle Actuator for Exoskeleton Arm in Post-Stroke Rehabilitation*, 2019.

- [67] Zhang GL, Lin MX, and Ieee, *Design of a Soft Robot Using Pneumatic Muscles for Elbow Rehabilitation*, 2018.
- [68] Deaconescu A and Deaconescu T, "Wrist Rehabilitation Equipment Based on the Fin-Ray (R) Effect," in *Advances in Service and Industrial Robotics*. vol. 980, K. Berns and D. Gorges, Eds., ed, 2020, p. 393-401.
- [69] Balasubramanian S, Huang H, and He J, "Quantification of dynamic property of pneumatic muscle actuator for design of therapeutic robot control," in *Int Conf IEEE Eng Med Biol*, New York, NY, USA, 2006, p. 2734.
- [70] Balasubramanian S, Ward J, Sugar T, and He J, "Characterization of the dynamic properties of pneumatic muscle actuators," in *IEEE Int Conf Rehab Rob*, Noordwijk, Netherlands, 2007, p. 764-770.
- [71] Tu X, He J, Wen Y, Huang J, Huang X, Huang H, *et al.*, "Cooperation of electrically stimulated muscle and pneumatic muscle to realize RUPERT bi-directional motion for grasping," *Conf Proc IEEE Eng Med Biol Soc*, vol. 2014, pp. 4103-4106, 2014.
- [72] Xiong C, Jiang X, Sun R, Huang XL, and Xiong Y, "Control methods for exoskeleton rehabilitation robot driven with pneumatic muscles," *Ind Robot*, vol. 36, pp. 210-220, 2013.
- [73] Prado GV and Sanchez MBC, "Control Strategy of a Pneumatic Artificial Muscle for an Exoskeleton Application," *Ifac Papersonline*, vol. 52, pp. 281-286, 2019.
- [74] Ahn KK and Tu DCT, "Nonlinear PID control to improve the control performance of the pneumatic artificial muscle manipulator using neural network," *J Mech Sci Tech*, vol. 19, pp. 106-115, 2005.
- [75] Anh HPH, Kien CV, and Nam NT, "Advanced force control of the 2-axes PAM-based manipulator using adaptive neural networks," *Robotica*, vol. 36, pp. 1333-1362, Sep 2018.
- [76] Anh HPH, Son NN, and Kien CV, "Adaptive Neural Compliant Force-Position Control of Serial PAM Robot," *Journal of Intelligent & Robotic Systems*, vol. 89, pp. 351-369, Mar 2018.
- [77] Jiang XZ, Huang XH, Xiong CH, Sun RL, and Xiong YL, "Position control of a rehabilitation robotic joint based on neuron proportion-integral and feedforward control," *J. Comput. Nonlinear*, vol. 7, p. 024502, 2012.
- [78] Chang MK, "An adaptive self-organizing fuzzy sliding mode controller for a 2-DOF rehabilitation robot actuated by pneumatic muscle actuators," *Control Eng Pract*, vol. 18, pp. 13-22, 2010.
- [79] Chang MK and Yuan TH, "Experimental implementations of adaptive self-organizing fuzzy slide mode control to a 3-DOF rehabilitation robot," in *Int Conf Innov Comput Inf Control*, Dalian, Liaoning, China, 2008, p. 503-503.
- [80] Chang MK, "Adaptive self-tuning fuzzy controller for a soft rehabilitation machine actuated by pneumatic artificial muscles," *Open J Appl Sci*, vol. 05, pp. 199-211, 2015.
- [81] Huang J, Qian J, Liu L, Wang Y, Xiong C, and Ri S, "Echo state network based predictive control with particle swarm optimization for pneumatic muscle actuator," *Journal of the Franklin Institute*, vol. 353, pp. 2761-2782, 2016.
- [82] Wu J, Huang J, Wang Y, and Xing K, "Nonlinear Disturbance Observer-Based Dynamic Surface Control for Trajectory Tracking of Pneumatic Muscle System," *IEEE T Contr Syst T*, vol. 22, pp. 440-455, 2014.
- [83] Huang J, Cao Y, Xiong CH, and Zhang HT, "An Echo State Gaussian Process-Based Nonlinear Model Predictive Control for Pneumatic Muscle Actuators," *IEEE Transactions on Automation Science and Engineering*, vol. 16, pp. 1071-1084, Jul 2019.
- [84] Qian J, Huang J, and Ri S, "Adaptive fuzzy sliding mode control for pneumatic muscle actuator," in *Chinese Automation Congress*, 2015, p. 431-436.
- [85] Liu H, "Pneumatic muscle actuator position control based on sliding mode control algorithms."
- [86] Hussain S, Xie SQ, and Jamwal PK, "Adaptive impedance control of a robotic orthosis for gait rehabilitation," *IEEE T Cy*, vol. 43, pp. 1025-1034, 2013.
- [87] Khajehsaeid H, Esmaeili B, Soleymani R, and Delkhosh A, "Adaptive back stepping fast terminal sliding mode control of robot manipulators actuated by pneumatic artificial muscles: continuum modelling, dynamic formulation and controller design," *Meccanica*, vol. 54, pp. 1203-1217, Jun 2019.
- [88] Dao QT and Yamamoto SI, "Assist-as-Needed Control of a Robotic Orthosis Actuated by Pneumatic Artificial Muscle for Gait Rehabilitation," *Applied Sciences-Basel*, vol. 8, Apr 2018.
- [89] Cao J, Xie SQ, and Das R, "MIMO sliding mode controller for gait exoskeleton driven by pneumatic muscles," *IEEE T Contr Syst T*, vol. 9, pp. 44-53, 2017.
- [90] Hussain S, Jamwal PK, Ghayesh MH, and Xie SQ, "Assist-as-needed control of an intrinsically compliant robotic gait training orthosis," *IEEE T Ind Electron*, vol. 64, pp. 1675-1685, 2017.
- [91] Cao Y, Huang J, Huang ZB, Tu XK, Ru HG, Chen C, *et al.*, "Dynamic Model of Exoskeleton based on Pneumatic Muscle Actuators and Experiment Verification," in *2018 Ieee-Ras 18th International Conference on Humanoid Robots*, T. Asfour, Ed., ed, 2018, p. 334-339.
- [92] Cao JH, Xie SQ, and Das R, "MIMO Sliding Mode Controller for Gait Exoskeleton Driven by Pneumatic Muscles," *Ieee Transactions on Control Systems Technology*, vol. 26, pp. 274-281, Jan 2018.
- [93] Ma Y, Xie SQ, and Zhang Y, "A patient-specific biological command based controller for the Human-inspired robotic exoskeleton (HuREx): A case study for gait-swing assistance robot," in *IEEE Int Conf Mech Autom*, Tianjin, China, 2014, p. 286-291.
- [94] Kora K, Lu CZ, and Mcdaid AJ, "Automatic tuning with feedforward compensation of the HuREx rehabilitation system," in *IEEE/ASME Int Conf AIM*, Besacon, France, 2014, p. 1504-1509.

- [95] Zhang MM, McDaid A, Veale AJ, Peng YX, and Xie SQ, "Adaptive Trajectory Tracking Control of a Parallel Ankle Rehabilitation Robot With Joint-Space Force Distribution," *IEEE Access*, vol. 7, pp. 85812-85820, 2019.
- [96] Ai QS, Zhu CX, Zuo J, Meng W, Liu Q, Xie SQ, *et al.*, "Disturbance-Estimated Adaptive Backstepping Sliding Mode Control of a Pneumatic Muscles-Driven Ankle Rehabilitation Robot," *Sensors*, vol. 18, Jan 2018.
- [97] Meng W, Xie SQ, Liu Q, Lu CZ, and Ai QS, "Robust Iterative Feedback Tuning Control of a Compliant Rehabilitation Robot for Repetitive Ankle Training," *IEEE/ASME Trans Mech*, vol. 22, pp. 173-184, Feb 2017.
- [98] Ai QS, Wang L, Chen K, Chen AQ, Hu JW, Fang YL, *et al.*, "Cooperative Control of An Ankle Rehabilitation Robot Based on Human Intention," in *2018 Joint Ieee 8th International Conference on Development and Learning and Epigenetic Robotics*, ed, 2018, p. 181-186.
- [99] Ganguly S, Garg A, Pasricha A, and Dwivedy SK, "Control of pneumatic artificial muscle system through experimental modelling," *Mechatronics*, vol. 22, pp. 1135-1147, 2012.
- [100] Sakthivelu V, Chong S-H, Tan MH, and Ghazaly MM, "Phenomenological Modeling and Classic Control of a Pneumatic Muscle Actuator System," *Int. J. Control. Autom*, vol. 9, pp. 301-312, 2016.
- [101] Anh HPH and Ahn KK, "Hybrid control of a pneumatic artificial muscle (PAM) robot arm using an inverse NARX fuzzy model," *Eng Appl Artif Intel*, vol. 24, pp. 697-716, 2011.
- [102] Zhang DH, Zhao XG, and Han JD, "Active Model-Based Control for Pneumatic Artificial Muscle," *IEEE T Ind Electron*, vol. 64, pp. 1686-1695, Feb 2017.
- [103] Fan J, Zhong J, Zhao J, and Zhu Y, "BP neural network tuned PID controller for position tracking of a pneumatic artificial muscle," *Technol Health Care*, vol. 2, pp. 231-248, 2015.
- [104] Xing K, Huang J, Wang Y, and Wu J, "Tracking control of pneumatic artificial muscle actuators based on sliding mode and non-linear disturbance observer," *Control Theor. A*, vol. 4, pp. 2058-2070, 2010.
- [105] Liu Q, Liu D, Meng W, Zhou Z, and Ai Q, "Fuzzy sliding mode control of a multi-DOF parallel robot in rehabilitation environment," *Int J Hum Rob*, vol. 11, 2014.
- [106] Bharadwaj K, Sugar TG, Koeneman JB, and Koeneman EJ, "Design of a robotic gait trainer using spring over muscle actuators for ankle stroke rehabilitation," *J Biomech Eng*, vol. 127, pp. 1009-1013, 2005.
- [107] Leephakpreeda T, "Mathematical modeling of pneumatic artificial muscle actuation via hydrogen driving metal hydride-LaNi5," *J Bionic Eng*, vol. 9, pp. 110-118, 2012.
- [108] Leephakpreeda T, "Fuzzy self-tuning PID control of hydrogen-driven pneumatic artificial muscle actuator," *J Bionic Eng*, vol. 10, pp. 329-340, 2013.
- [109] Belforte G, Eula G, Ivanov A, Raparelli T, and Sirolli S, "Presentation of textile pneumatic muscle prototypes applied in an upper limb active suit experimental model," *Journal of the Textile Institute*, vol. 109, pp. 757-766, 2018.
- [110] Zhou XL and Jiang XM, *Analysis And Research Based on Soft Bending Pneumatic Actuator*, 2019.
- [111] Giovacchini F, Vannetti F, Fantozzi M, Cempini M, Cortese M, Parri A, *et al.*, "A light-weight active orthosis for hip movement assistance," *Robot Auton Syst*, vol. 73, pp. 123-134, 2015.
- [112] Noda T, Takai A, Teramae T, Hirooka E, Hase K, Morimoto J, *et al.*, "Robotizing Double-Bar Ankle-Foot Orthosis," in *2018 Ieee International Conference on Robotics and Automation*, ed, 2018, p. 2782-2787.
- [113] Al-Fahaam H, Davis S, and Nefti-Meziani S, "The design and mathematical modelling of novel extensor bending pneumatic artificial muscles (EBPAMs) for soft exoskeletons," *Robotics and Autonomous Systems*, vol. 99, pp. 63-74, Jan 2018.
- [114] Seo YS, Cho SJ, Lee JY, Park C, Kim U, Lee S, *et al.*, "Human-mimetic soft robot joint for shock absorption through joint dislocation," *Bioinspiration & Biomimetics*, vol. 15, Jan 2020.
- [115] Laski PA, Zwierzchowski J, and Pietrala DS, "Development of Delta-Type Parallel Robot Using Pneumatic Artificial Muscles in Application for Rehabilitation," in *Engineering Mechanics 2018 Proceedings, Vol 24*, C. Fischer and J. Naprstek, Eds., ed, 2018, p. 489-492.
- [116] Kora K, McDaid A, and Xie S, "Non-linear model-based Control for the Human-inspired Robotic Exoskeleton (HuREx) gait trainer," *Ifac Papersonline*, vol. 47, pp. 11830-11835, 2014.
- [117] Nichols M TN, Luengo-Fernandez R, Leal J, Gray A, Scarborough P, Rayner M (2012), "European Cardiovascular Disease Statistics 2012," *European Heart Network, Brussels, European Society of Cardiology, Sophia Antipolis*, 2012.
- [118] Pitel' J and Tóthová M, "Modelling of pneumatic muscle actuator using Hill's model with different approximations of static characteristics of artificial muscle," in *Int Conf Circ Syst Commun Comput*, Corfu Island, Greece, 2016, p. 02015.
- [119] Cortese M, Cempini M, De AR, P. R, and Soekadar SR, "A mechatronic system for robot-mediated hand telerehabilitation," *IEEE/ASME Trans Mech*, vol. 20, pp. 1753-1764, 2014.
- [120] Novak D and Riener R, "A survey of sensor fusion methods in wearable robotics," *Robot Auton Syst*, vol. 73, pp. 155-170, 2015.
- [121] Saito N, "Effects on knee joint force from a body weight load reduction system driven by rubber-less artificial muscle," *Industrial Robot: the international journal of robotics research and application*, vol. 46, pp. 642-649, 2019.
- [122] Tang Z, Sun S, Zhang S, Chen Y, Li C, and Chen S, "A brain-machine interface based on ERD/ERS for an upper-limb exoskeleton control," *Sensors*, vol. 16, p. 2050, 2016.
- [123] Looned R, Webb J, Xiao ZG, and Menon C, "Assisting drinking with an affordable BCI-controlled wearable robot and electrical stimulation: a preliminary investigation," *J Neuroeng Rehab*, vol. 11, pp. 1-13, 2014.

- [124] Johansson BB, "Current trends in stroke rehabilitation. A review with focus on brain plasticity," *Acta Neurol Scand*, vol. 123, pp. 147-159, 2011.
- [125] Simonetti D, Zollo L, Papaleo E, Carpino G, and Guglielmelli E, "Multimodal adaptive interfaces for 3D robot-mediated upper limb neuro-rehabilitation," *Robot Auton Syst*, vol. 85, pp. 62-72, 2016.
- [126] Chen K, Ren Y, Gaebler-Spira D, and Zhang LQ, "Home-based tele-assisted robotic rehabilitation of joint impairments in children with cerebral palsy," in *Eng Med Biol Soc*, 2014, p. 5288-5291.
- [127] Mazzoleni S, Turchetti G, Palla I, Posteraro F, and Dario P, "Acceptability of robotic technology in neuro-rehabilitation: Preliminary results on chronic stroke patients," *Comput Methods Prog Biomed*, vol. 116, pp. 116-122, 2014.
- [128] Mazzoleni S, Puzzolante L, Zollo L, Dario P, and Posteraro F, "Mechanisms of motor recovery in chronic and subacute stroke patients following a robot-aided training," *IEEE T Haptics IEEE T. Haptics.*, vol. 7, pp. 175-180, 2013.
- [139] Contrerasvidal JL and Grossman RG, "NeuroRex: A clinical neural interface roadmap for EEG-based brain machine interfaces to a lower body robotic exoskeleton," in *IEEE Int Conf EMBC*, Osaka, Japan, 2013, p. 1579-1582.
- [130] Onose G, Grozea C, Anghelescu A, Daia C, Sinescu C, Ciurea A, *et al.*, "On the feasibility of using motor imagery EEG-based brain-computer interface in chronic tetraplegics for assistive robotic arm control: a clinical test and long-term post-trial follow-up," *Spinal Cord*, vol. 50, pp. 599-608, 2012.
- [131] Stampacchia G, Mazzoleni S, Rustici A, Bigazzi S, Gerini A, and Tombini T, "Walking with a powered robotic exoskeleton: Subjective experience, spasticity and pain in spinal cord injured persons," *Neurorehabilitation*, vol. 39, pp. 277-283, 2016.
- [132] Shirota C, Jansa J, Diaz J, Balasubramanian S, Mazzoleni S, Borghese NA, *et al.*, "On the assessment of coordination between upper extremities: towards a common language between rehabilitation engineers, clinicians and neuroscientists," *J Neuroeng Rehab*, vol. 13, p. 80, 2016.
- [133] Lin CJ, Lin CR, Yu SK, and Chen CT, "Hysteresis modeling and tracking control for a dual pneumatic artificial muscle system using Prandtl-Ishlinskii model," *Mechatronics*, vol. 28, pp. 35-45, 2015.



Quan Liu received the Ph.D. degree in mechanical manufacturing & Automation, in 2004 from Wuhan University of Technology, Wuhan, China. She is currently a Professor at Wuhan University of Technology. During recent years, she authored more than 60 technical publications, proceedings, editorials, and books. She has directed more than 20 research projects. Her research interests include signal processing, embedded systems, and robots and electronics.

Dr. Liu received two national awards and three provincial and ministerial awards. She was awarded as the "National Excellent Teacher" in 2007. She is a Council Member of the Chinese Association of Electromagnetic Compatibility and the Hubei Institute of Electronics.



Jie Zuo received the B.S. degree in information engineering from Wuhan University of Technology, Wuhan, China, in 2015. Since 2016, she has been studying as a student with successive postgraduate and doctoral programs at Wuhan University of Technology. She has directed one research projects and participated in more than 3 research projects in areas of rehabilitation robots dynamic modelling and motion control.



Chang Zhu received the B.S. degree in information engineering from Wuhan University of Technology, Wuhan, China, in 2019. Since 2020, he has been studying as a student with postgraduate at Wuhan University of Technology. His current research interests include wearable robotics, robot motion control, and robotics for lower limb rehabilitation.



Sheng Q. Xie received his Ph.D. degrees from Huazhong University of Science and Technology, China and University of Canterbury, New Zealand, in 1998 and 2002, respectively. He joined University of Auckland in 2003 and became a Chair Professor in (bio)mechatronics in 2011. Since 2017 he has been the Chair Professor in Robotics and Autonomous Systems at the University of Leeds. He has published 7 books, 15 book chapters, and over 400 international journal and conference papers. His current research interests are medical and rehabilitation robots, advanced robot control. Prof. Xie is an elected Fellow of The Institution of Professional Engineers New Zealand (FIPENZ). He has also served as a Technical Editor for IEEE/ASME TRANSACTIONS ON MECHATRONICS.

