



UNIVERSITY OF LEEDS

This is a repository copy of *Does a novel X-ray imaging technology provide a substantial radiation dose reduction for patients in trans-catheter aortic valve implantation procedures?*.

White Rose Research Online URL for this paper:
<http://eprints.whiterose.ac.uk/84812/>

Version: Published Version

Conference or Workshop Item:

Gislason-Lee, AJ, Blackman, D and Davies, AG (2014) Does a novel X-ray imaging technology provide a substantial radiation dose reduction for patients in trans-catheter aortic valve implantation procedures? In: UNSPECIFIED, 22 Oct 2014, British Institute of Radiology. (Unpublished)

Reuse

Unless indicated otherwise, fulltext items are protected by copyright with all rights reserved. The copyright exception in section 29 of the Copyright, Designs and Patents Act 1988 allows the making of a single copy solely for the purpose of non-commercial research or private study within the limits of fair dealing. The publisher or other rights-holder may allow further reproduction and re-use of this version - refer to the White Rose Research Online record for this item. Where records identify the publisher as the copyright holder, users can verify any specific terms of use on the publisher's website.

Takedown

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing eprints@whiterose.ac.uk including the URL of the record and the reason for the withdrawal request.



eprints@whiterose.ac.uk
<https://eprints.whiterose.ac.uk/>

Does a novel X-ray imaging technology provide a substantial radiation dose reduction for trans-catheter aortic valve implantation (TAVI) patients?

Amber J. Gislason-Lee, Daniel Blackman*, Andrew G. Davies

Division of Medical Physics, University of Leeds, UK; *Cardiology Department, Leeds General Infirmary, UK



Introduction

Trans-catheter aortic valve implantation (TAVI) is a treatment for patients with symptomatic aortic stenosis, who are high risk or inoperable for conventional surgical aortic valve replacement. A dynamic interventional X-ray imaging system is used to visualize treatment in real time. The resulting patient radiation dose is amongst the highest from medical imaging procedures¹, and operator doses are the highest of all interventional cardiac procedures². The X-ray system must minimise radiation dose whilst maintaining adequate image quality for the clinical task, as per the ALARP principle³.

Modern interventional X-ray equipment employs image processing to permit such a reduction in radiation dose. The aim of this study was to investigate whether our recently-installed system (AlluraClarity, Philips Healthcare) which contains advanced real-time image noise reduction algorithms and anatomy-specific X-ray optimization, affected patient procedure dose and fluoroscopy duration in routine TAVI procedures.

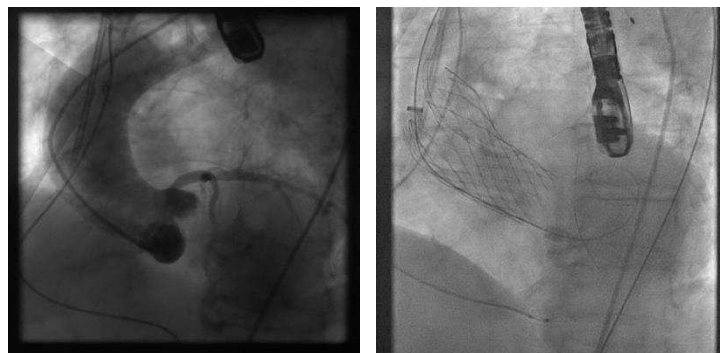




Image frame from (left) baseline aortogram and (right) final release of valve

Methods


Procedures done for 42 TAVI patients from the AlluraClarity cardiac catheter lab and from a reference system (Axiom Artis, Siemens Healthcare) in the same cardiology department were recorded. Median values from the two X-ray systems were compared using the Wilcoxon statistical test.

Results

Total procedure dose medians were 4016 and 7088 cGy cm² from the AlluraClarity and reference systems respectively. Fluoroscopy and digital image acquisition ('cine') contributions are shown in figures below with fluoroscopy duration. All differences in patient dose were significant at the 5% level.

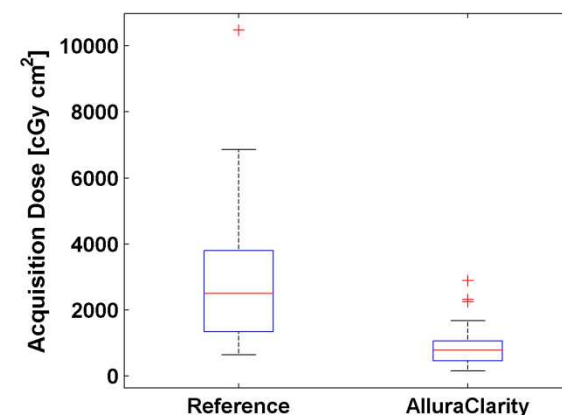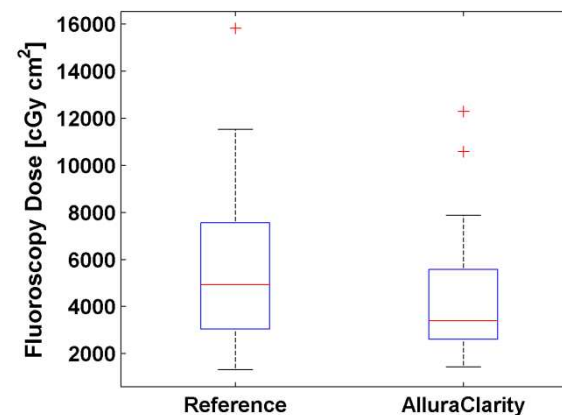

Figures: red line is median, blue box is first and third quartiles, black is minimum and maximum values and red +'s are outliers.

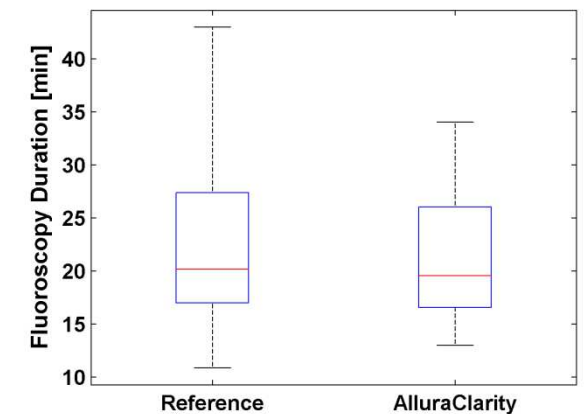

Conclusions

The AlluraClarity cardiac catheter lab had 43% lower total patient procedure dose for TAVI patients than the reference lab. Fluoroscopy and digital image acquisition doses were 31% and 69% lower respectively, with no statistically significant difference in fluoroscopy duration between the two labs.

Acknowledgements

This project was supported by Philips Healthcare, The Netherlands.

References

- ¹Sharma D, Ramsewak S, O'connaire R, Verghis G, Manoharan MS. Radiation exposure reduction during transcatheter aortic valve implantation (TAVI) procedures. *Heart* 99, A34 (2013).
- ²Drury-Smith M, Maher A, Douglas-Hill C, Singh R, Bhabra M, Cotton J, Khogali S, TAVI operators radiation dose compared to PCI and ICD operators: Do we need additional radiation protection for trans-catheter structural heart interventions, *Heart* 97, Suppl1 (2011).
- ³ICRP. Avoidance of radiation injuries from medical interventional procedures. ICRP Publication 85. *Ann ICRP* 30(2) (2000).