



This is a repository copy of *Recognition of walking activity and prediction of gait periods with a CNN and first-order MC strategy*.

White Rose Research Online URL for this paper:
<http://eprints.whiterose.ac.uk/139218/>

Version: Accepted Version

Proceedings Paper:

Martinez-Hernandez, U., Rubio-Solis, A. and Dehghani-Sanij, A.A. (2018) Recognition of walking activity and prediction of gait periods with a CNN and first-order MC strategy. In: Proceedings of the IEEE International Conference on Biomedical Robotics and Biomechatronics (Biorob). 2018 7th IEEE International Conference on Biomedical Robotics and Biomechatronics (Biorob), 26-29 Aug 2018, Enschede, Netherlands. IEEE , pp. 897-902. ISBN 9781538681831

<https://doi.org/10.1109/BIOROB.2018.8487220>

© 2018 IEEE. Personal use of this material is permitted. Permission from IEEE must be obtained for all other users, including reprinting/ republishing this material for advertising or promotional purposes, creating new collective works for resale or redistribution to servers or lists, or reuse of any copyrighted components of this work in other works. Reproduced in accordance with the publisher's self-archiving policy.

Reuse

Items deposited in White Rose Research Online are protected by copyright, with all rights reserved unless indicated otherwise. They may be downloaded and/or printed for private study, or other acts as permitted by national copyright laws. The publisher or other rights holders may allow further reproduction and re-use of the full text version. This is indicated by the licence information on the White Rose Research Online record for the item.

Takedown

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing eprints@whiterose.ac.uk including the URL of the record and the reason for the withdrawal request.



eprints@whiterose.ac.uk
<https://eprints.whiterose.ac.uk/>

Recognition of walking activity and prediction of gait periods with a CNN and first-order MC strategy

Uriel Martinez-Hernandez, Adrian Rubio-Solis and Abbas A. Dehghani-Sanij

Abstract—In this paper, a strategy for recognition of human walking activities and prediction of gait periods using wearable sensors is presented. First, a Convolutional Neural Network (CNN) is developed for the recognition of three walking activities (level-ground walking, ramp ascent and descent) and recognition of gait periods. Second, a first-order Markov Chain (MC) is employed for the prediction of gait periods, based on the observation of decisions made by the CNN for each walking activity. The validation of the proposed methods is performed using data from three inertial measurement units (IMU) attached to the lower limbs of participants. The results show that the CNN, together with the first-order MC, achieves mean accuracies of 100% and 98.32% for recognition of walking activities and gait periods, respectively. Prediction of gait periods are achieved with mean accuracies of 99.78%, 97.56% and 97.35% during level-ground walking, ramp ascent and descent, respectively. Overall, the benefits of our work for accurate recognition and prediction of walking activity and gait periods, make it a suitable high-level method for the development of intelligent assistive robots.

I. INTRODUCTION

Recognition of activities of daily living (ADLs) is an important capability required in autonomous systems to deliver safe and accurate assistance to humans [1], [2]. Activities such as walking, ramp ascent/descent and sit-to-stand provide independence of living and transportation across different terrains, which make them particularly important for research of computational recognition methods [3], [4], [5].

In recent years, a rapid progress has been observed in sensor technology for collection of multimodal data measurements from human motion. Sensors have become wearable and lightweight, with modules integrated to provide inertial measurements and soft kinematic data [6], [7], [8]. Even though the rapid advancement on sensors, robust and accurate computational methods for the analysis and recognition of human motion are still under development [9], [10].

In this work, a strategy composed of a Convolutional Neural Network (CNN) and a first-order Markov Chain (MC), is presented for both, recognition of walking activity and prediction of gait periods. The recognition of level-ground walking, ramp ascent and descent activities is im-

This work was supported by the EPSRC for the project ‘Wearable soft robotics for independent living’ (EP/M026388/1).

Uriel Martinez-Hernandez is with the Department of Electronic and Electrical Engineering, the University of Bath, Bath, BA2 7AY, U.K. (email: u.martinez@bath.ac.uk)

Adrian Rubio-Solis is with the Department of Automatic Control and Systems Engineering, the University of Sheffield, Sheffield, S1 3JD, U.K. (email: a.rubiosolis@sheffield.ac.uk)

Abbas A. Dehghani-Sanij is with the School of Mechanical Engineering, the University of Leeds, Leeds, LS2 9JT, U.K. (email: a.a.dehghani-sanij@leeds.ac.uk)

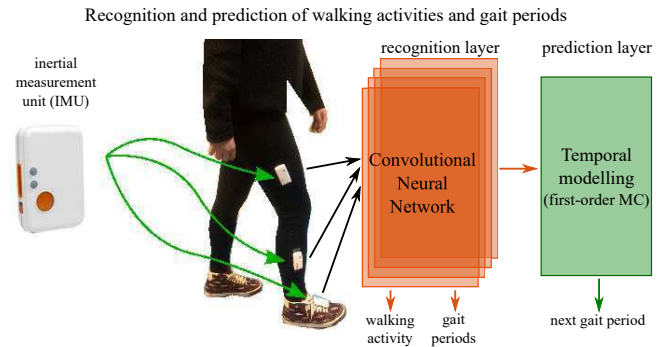


Fig. 1. High-level method, composed of a CNN and first-order MC, for recognition and prediction of walking activities and gait periods. Real data collected from wearable sensors attached to the lower limbs of participants.

plemented with a CNN [11], [12]. In addition, this neural network is able to recognise the gait periods (initial contact, loading response, mid-stance, terminal stance, pre-swing, initial swing, mid-swing and terminal swing) and phases (stance and swing) that compose the human gait cycle. A temporal modelling, with a first-order MC [13], [14], is used for prediction of gait periods based on the observation, over time, of decisions made by the CNN for each walking activity. The proposed strategy is validated with multiple repetitions of three walking activities (level-ground walking, ramp ascent and descent), performed by participants wearing three inertial measurement unit (IMU) sensors attached to their lower limbs (Figure 1). The validation process uses real data, composed of angular velocity, accelerometer and magnetometer signals, collected from the thigh, shank and foot from each walking activity.

The experiments show that the CNN is capable to achieve mean accuracies of 100% for recognition of walking activities, 98.32% for gait periods, 97.42% for stance phase and 99.83% for swing phase. The first-order MC is able to predict gait periods with mean accuracies of 99.78%, 97.56% and 97.35% for level-ground walking, ramp ascent and descent. This information is important to know the probability of the next gait period and phase during the gait cycle. The recognition and prediction functionalities, provided by the proposed combination of high-level methods, are crucial for multi-layer architectures required for learning, interaction and control of autonomous assistive robots [15], [16], [17].

Overall, the results from the experiments show that the strategy composed of a CNN and first-order MC is highly accurate, which makes it suitable for the development of intelligent wearable robots capable to assist humans in ADLs.

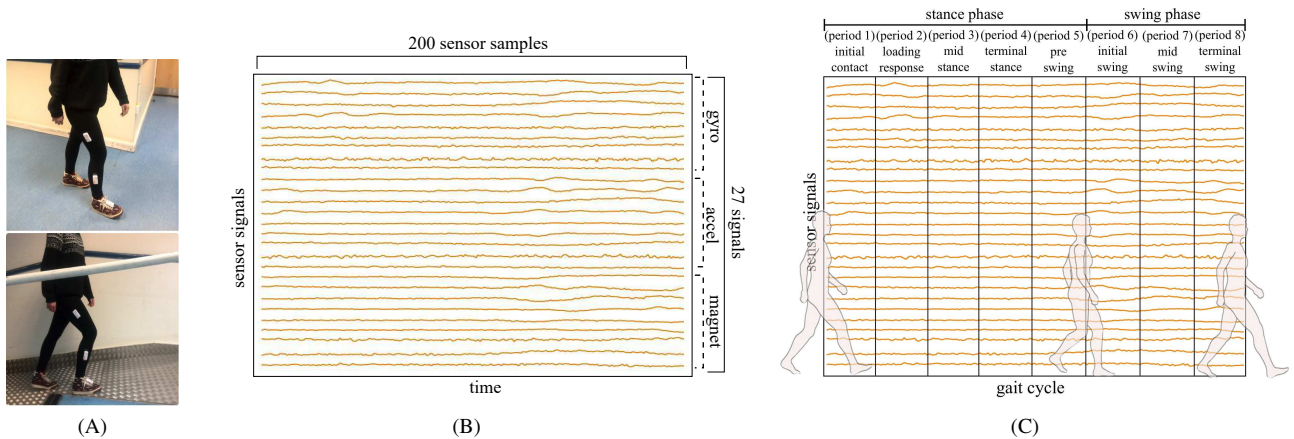


Fig. 2. Sensor signals for recognition and prediction of walking activities and gait periods. (A) Data collection from 9-DoF inertial measurement units (IMU) attached to the thigh, shank and foot. (B) Example of concatenated signals from gyroscope (x,y,z), accelerometer (x,y,z) and magnetometer (x,y,z) for a walking activity. (C) Segmentation of the dataset, into 8 periods, for recognition and prediction of gait periods and phases during a walking activity.

II. METHODS

A. Experimental protocol and data collection

Angular velocity, accelerometer and magnetometer signals were employed from three inertial measurement units (IMU), worn by 12 healthy human participants (Figure 1). Anthropometric data from participants are as follows: ages between 24 and 34 years old, heights between 1.70 m and 1.82 m, and weights between 75.5 kg and 88 kg.

Participants were asked to walk at their self-selected speed and perform ten repetitions of three walking activities: level-ground walking, ramp ascent and ramp descent (Figure 2A). Level-ground walking was performed on a flat cement surface. A metallic ramp, with a slope of 8.5 deg, was used for ramp ascent and descent. Sensor signals were systematically collected and filtered with a cut-off frequency of 10 Hz. For this process employed three IMUs (Shimmer Inc.) attached to the thigh, shank and foot of participants. For each IMU, angular velocity, accelerometer and magnetometer signals, in x - y and z axes, were sampled at 100 Hz. These signals were concatenated to form datasets, composed of 27 signals (3 signals \times 3 axes \times 3 sensors) and 200 sensor samples, from each activity performed by participants. Datasets from 8 and 4 participants were used to train and test the proposed strategy, respectively. Figure 2B shows an example of the signals collected from the wearable sensors during a walking activity. In addition, two foot pressure-insole sensors were used to detect the beginning and end of each gait cycle.

Figure 2C presents the segmentation of the gait cycle into stance phase, swing phase and eight periods (initial contact, loading response, mid-stance, terminal stance, pre-swing, initial swing, mid-swing, terminal swing). This segmentation allows the proposed strategy to recognise and predict the state of the human body during a walking activity.

B. CNN for recognition of walking activity and gait period

Convolutional Neural Networks (CNN) have shown their potential for speech recognition and image classification [18], [19], [20]. Here, a CNN is developed for recognition of walking activity and gait periods, using data

from wearable sensors. The proposed CNN model is presented in Figure 3A. The first layer uses 32 kernels of sizes 5×5 and 2×2 for convolution and max-pooling. The second layer uses 16 kernels of sizes 3×3 and 2×2 for convolution and max-pooling. Features from the second layer, which are flattened and fully connected, are used by the softmax layer to estimate the probability of the current walking activity and gait period. The CNN model receives input data from all walking activities, arranged in matrices of 27 signals \times 25 samples based on the segmentation into 8 periods of the complete activity matrix (27×200 , see Figure 2). This approach allows to recognise the walking activity and gait period performed by participants, e.g., level-ground walking and period 5 (pre-swing). The output map from each convolutional layer is obtained as follows:

$$x_{ij}^l = b_j + \sum_{a=0}^{m-1} \sum_{b=0}^{m-1} k_{ab} * y_{(i+a)(j+b)}^{l-1} \quad (1)$$

where x_{ij}^l is the output of the l layer of the j -th feature map on the i -th unit, and b_j is the bias. The operator $*$ denotes the convolution between the $m \times m$ kernel k_{ab} and the nonlinear output $y_{(i+a)(j+b)}^{l-1}$ from layer $l-1$. The nonlinear function σ is applied to the output from Equation (1) as follows:

$$y_{ij}^l = \sigma(x_{ij}^l) \quad (2)$$

where y_{ij}^l is the nonlinear output from the l convolutional layer and σ is the hyperbolic tangent function \tanh . A downsampling process is performed with a max-pooling layer after each convolutional layer. This process takes a $u \times u$ region (2×2 size in our CNN model) and provides the maximum value from that region as follows:

$$y_{ij}^l = \max_{u \times u} (y_{ij}^{l-1}) \quad (3)$$

where y_{ij}^l contains the maximum values from the nonlinear output y_{ij}^{l-1} . The process performed by convolutional and max-pooling layers is known as feature learning. The learned features, connected to a 1-dimensional feature vector y_c , are used by a softmax layer for classification, as follows:

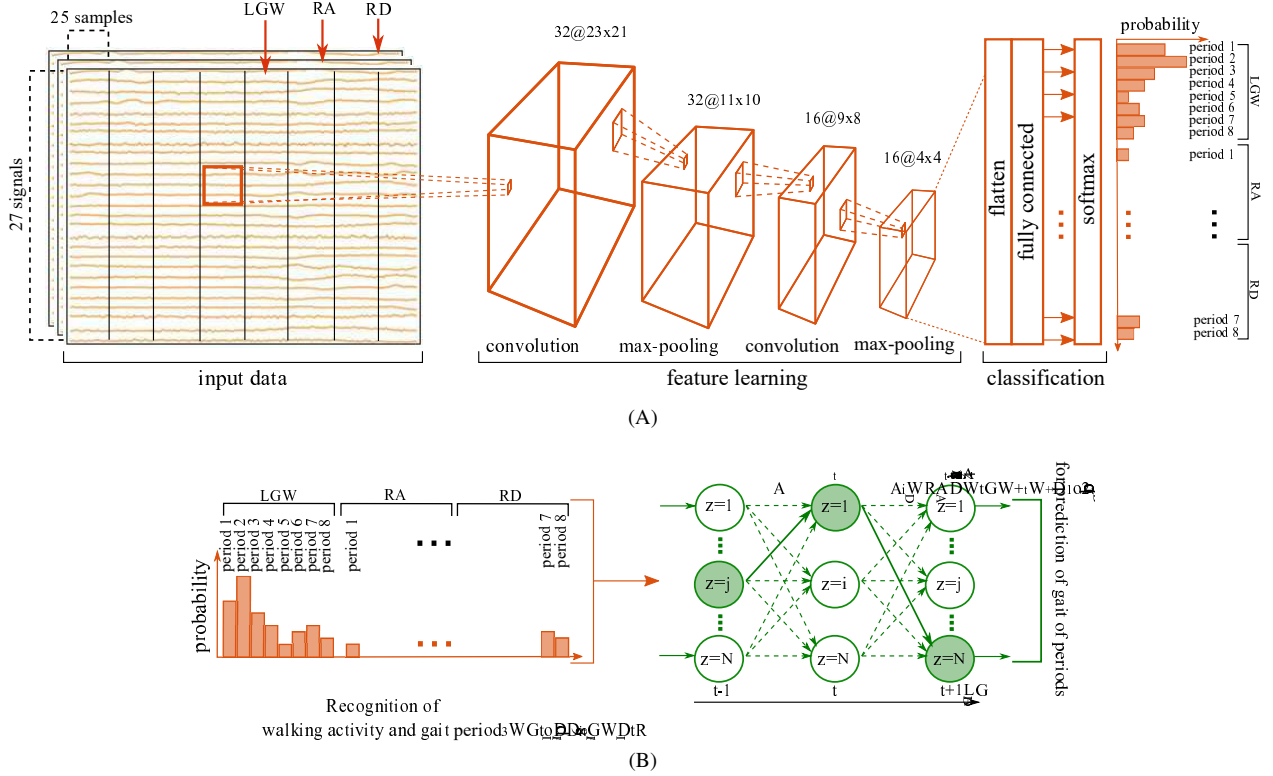


Fig. 3. CNN and first-order MC strategy for recognition and prediction of walking activities and gait periods using wearable sensors. (A) The CNN model is composed of two convolutional and max-pooling layers, followed by flatten, fully connected and softmax layers. Input sensor data from all walking activities (level-ground walking (LGW), ramp ascent (RA) and ramp descent (RD)) are segmented into 8 periods (initial contact, loading response, mid-stance, terminal stance, pre-swing, initial swing, mid-swing and terminal swing). The CNN estimates the current walking activity and gait period performed by a participant. (B) The first-order MC predicts the next gait period based on the observation of current recognition decisions from the CNN.

$$P(c|y) = \frac{e^{y^T w_c}}{\sum_{n=1}^N e^{y^T w_n}} \quad (4)$$

$$\hat{c} = \arg \max_c P(c|y) \quad (5)$$

where $P(c|y)$ contains the probabilities for all classes (walking activities and gait periods), given the sample vector y . The parameters w and N represent the weight vector and total number of classes, respectively. In Equation (5), the recognition of the current walking activity and gait period, \hat{c} , is obtained with the *maximum a posteriori* (MAP) estimate.

The output from the CNN allows to know the state of the human body while performing walking activities. This information is needed for control of assistive and rehabilitation robots, but also is important for prediction of gait periods during the current walking cycle. An approach for prediction of gait periods is presented in the next Section II-C.

C. First-order MC for prediction of gait periods

The prediction of gait periods is based on the sequential analysis of decisions made by the CNN. Markov models are useful to model sequential data and assume that future predictions are independent of all but the most recent observations. Specifically, here, a first-order Markov Chain (MC) of observations is employed, where the probability distribution $P(z_t|z_{t-1})$ of a particular observation z_t at time t is conditioned on the observation z_{t-1} at time $t-1$. The

directed graph in Figure 3B shows the first-order MC, which receives the gait period, z_t , recognised by the CNN. The joint distribution for a sequence of T observations is given by:

$$P(z_1, \dots, z_T) = P(z_1) \prod_{t=2}^T P(z_t|z_{t-1}) \quad (6)$$

In Equation (6), the conditional probability distribution for observation z_t , given the d-separation property and all observations up to time t , is obtained as follows:

$$P(z_t|z_1, \dots, z_{t-1}) = P(z_t|z_{t-1}) \quad (7)$$

The temporal models in Equation (7) predicts the next observation in a sequence using only the immediately preceding observation [21]. However, there is no standard procedure for an efficient application [22], [23]. Here, online implementation of MC for prediction of the next observation z_{t+1} , is based on the algorithm presented in [24], as follows:

$$P(z_{t+1}) = A_t P(z_t) \quad (8)$$

where z_t is a random variable with N states, $P(z_{t+1})$ is the predicted state, $P(z_t) = [P(z_t) = 1, \dots, P(z_t) = N]$ is a stochastic state vector and $A_t = [a_{ij_t}]$, with $i, j = 1 \dots N$, is a time-dependent transition matrix. The state vector is recursively updated by estimates of A_t , as follows:

$$a_{ij_t} = \rho \Gamma_{ij_t}, \quad i, j = 1, \dots, N \quad (9)$$

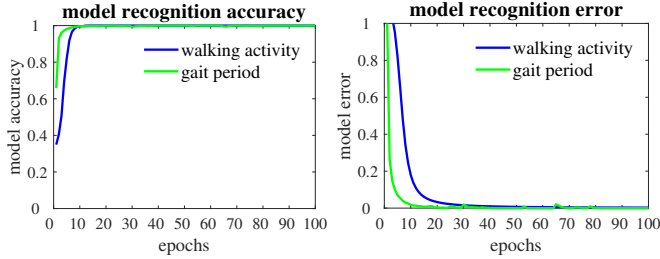


Fig. 4. Training results of the CNN for recognition of walking activity (blue colour curve) and gait period (green colour curve). (left) Accuracy and (right) error recognition results achieved by the CNN method.

$$\Gamma_{ij_t} = \left(\frac{t-1}{t}\right) \Gamma_{ij_{t-1}} + \left(\frac{1}{t}\right) \zeta_{ij} \quad (10)$$

where ρ is a normalising factor and Γ_{ij_t} is the transition likelihood of the j -th state at $t-1$ to the i -th state at time t . The variable ζ_{ij_t} is updated as follows:

$$\zeta_{ij_t} = \begin{cases} \hat{c}_t & \text{if } P(z_t = i | z_{t-1} = j) \\ 0 & \text{otherwise} \end{cases} \quad (11)$$

$$\tilde{c} = \arg \max_z P(z_{t+1}) \quad (12)$$

where ζ_{ij_t} takes the value zero or \hat{c}_t , which is the probability of the gait period at time t from the CNN. Finally, the MAP estimate is applied to $P(z_{t+1})$ to obtain the predicted state or gait period, \tilde{c} , for next time $t+1$ during the walking activity.

III. RESULTS

The CNN and first-order MC strategy is validated with the recognition of walking activity and gait periods, and prediction of gait periods. For this process, training and testing datasets were collected from IMUs attached to the thigh, shank and foot of participants (see Section II-A).

A. Recognition of walking activity and gait periods

First, the accuracy of the high-level recognition of walking activities and gait periods was validated. This experiment employed angular velocity, accelerometer and magnetometer signals from level-ground walking, ramp ascent and descent activities. An example of these signals, measured from the thigh, shank and foot of participants, is shown in Figure 2B. The gait periods (initial contact, loading response, mid-stance, terminal stance, pre-swing, initial swing, mid-swing and terminal swing) in which the gait cycle was divided for recognition and prediction are shown in Figure 2C. Sensor datasets from 12 participants were split in two groups of 8 and 4 to train and test the high-level method, respectively.

The CNN model was configured to recognise 24 classes. The first group of 8 classes represents the eight gait periods for level-ground walking. The second group of 8 classes are the eight gait periods for ramp ascent. The third group of 8 classes corresponds to the eight gait periods for ramp descent. The architecture of the proposed CNN model is shown in Figure 3A. The model accuracy and error, randomly

drawing sensor samples from the training datasets, are shown in Figures 4A and 4B. These results show that, in the training step, the CNN required 100 epochs to achieve the mean accuracy of 100% for both, recognition of walking activity (blue colour curve) and gait period (green colour curve). Similarly, in the training step, the CNN model required 100 epochs to achieve the smallest error of 0% for recognition for walking activity and gait period. Sensor samples, randomly drawn from the testing datasets, were used to evaluate the CNN with new data. This process achieved an accuracy of 100% for recognition of individual walking activities (Figure 5A). The mean accuracy of 98.32% for recognition of gait periods for all walking activities is shown in Figure 5B. From these results, it is observed that recognition of stance (periods 1 to 5) and swing (periods 6 to 8) phases are 97.42% and 99.83%, respectively (Figure 5C). The recognition of gait periods and phases is important to know the state of the human body during the gait cycle, e.g., heel contact and toe-off. The accuracy recognition of gait periods for individual walking activities are shown in Figures 5D, 5E, and 5F. These results show that the CNN was able to recognise gait periods for level-ground walking, ramp ascent and descent with accuracies of 99.92%, 97.62% and 97.43%, respectively.

B. Prediction of gait periods

Prediction of gait periods allows to know the probability for the next gait period during the walking cycle, which is important for a better control of assistive robots. The results from prediction of gait periods, using the first-order MC temporal model, are shown in the confusion matrices of Figure 6. In this process, the MC model used the recognition output from the CNN during the walking activity. Then, the transition over time of gait periods was observed and learned by the MC model to estimate the next probable gait period. In Figure 6, the gait periods recognised by the CNN are shown in orange colour, while the estimated predictions from the MC are shown in grey scale colours. The confusion matrix in Figure 6A shows the prediction of gait periods for level-ground walking activity, where a mean accuracy of 99.78% was achieved. Similarly, Figures 6B and 6C show the mean gait period prediction accuracies of 97.56% and 97.35% for ramp ascent and ramp descent activities, respectively. Then, the first-order MC model was able to predict gait periods for all walking activities with a mean accuracy of 98.23%.

The results show that the performance of the prediction process, using the first-order MC, depends on the recognition accuracy of the CNN model. For that reason, prediction of gait periods for level-ground walking is more accurate than the results achieved for ramp ascent and descent. This prediction process is important to allow assistive robots to understand not only the current state of the human body, but also to perceive what is the next expected event during the walking activity. For instance, prediction of the swing phase is possible based on the recognition of gait periods during the stance phase. This predictive capability allows robots to be prepared for an expected event, and thus, delivering the needed assistance at the appropriate time in ADLs.

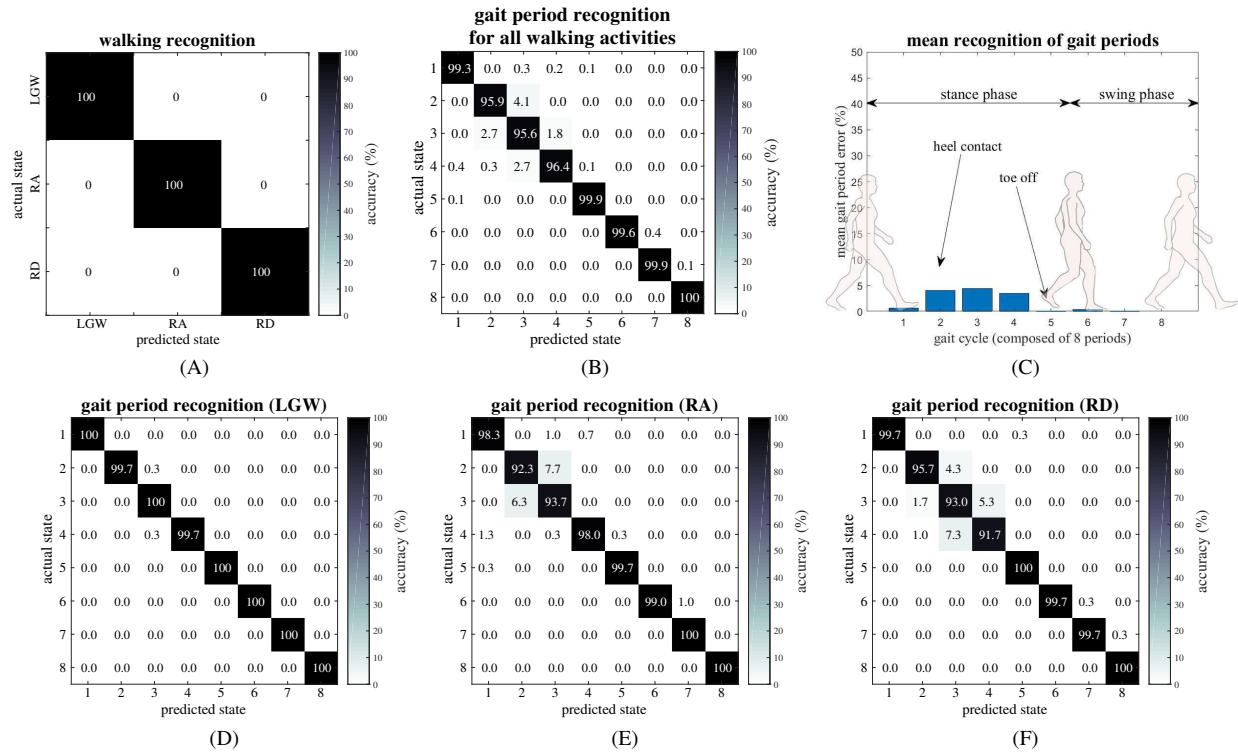


Fig. 5. Accuracy achieved by the CNN for recognition of walking activity and gait period using testing datasets. Low (0%) and high (100%) accuracy are represented by white and black colours, respectively. (A) Recognition accuracy for all walking activities. (B) Mean recognition accuracy of gait period for all walking activities. (C) Mean error recognition of gait periods and phases for all walking activities. Stance and swing phases correspond to periods 1 to 5 and 6 to 8, respectively. Recognition accuracy of gait periods for (D) level-ground walking, (E) ramp ascent and (F) ramp descent.

A comparison of the performance between the proposed strategy and state-of-the-art methods is presented in Table I. All methods are able to recognise walking activities with high accuracies ranging from 98% (DNB [30]) to 100% (GMM [28] and our CNN+first-order MC). Only a few methods are able to recognise gait periods and events with accuracies of 95.25% (DBN [30]), 97% (SVM [29]) and 98.32% (CNN + first-order MC), where the highest accuracy is achieved by our work. Our proposed strategy allows the prediction of gait periods (98.23%), which contrasts with the capabilities offered by all methods in Table I.

This comparative analysis shows the benefits of combining convolutional neural networks and Markov Chain models, together with wearable sensors, for robust recognition and prediction of walking activities and gait periods.

Overall, the results from all experiments showed the capability of the CNN and first-order MC strategy to perform high-level recognition and prediction processes. Thus, this work offers a suitable computational approach that, connected to mid- and low-level processes, has the potential to allow wearable robots to not only identify human motion, but also to provide reliable assistance in ADLs.

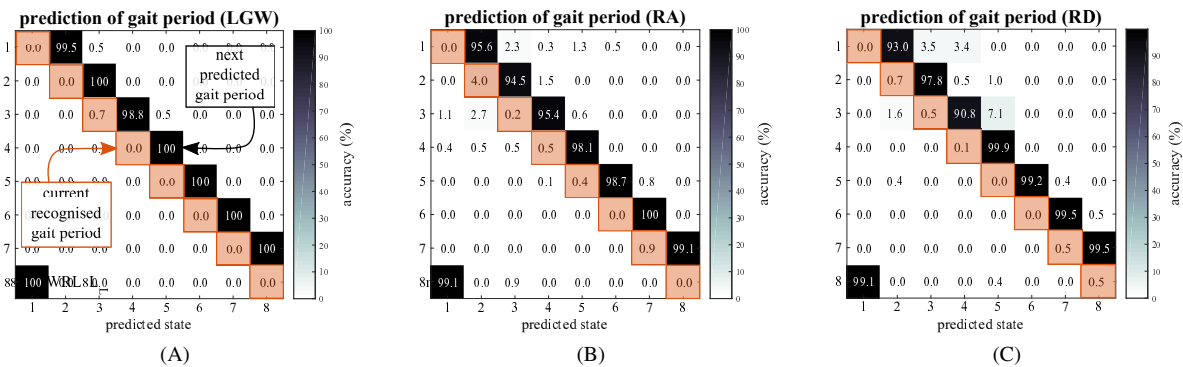


Fig. 6. Confusion matrices with the accuracy, achieved by the first-order MC, for prediction of gait periods for each of walking activity using testing datasets. Low (0%) and high (100%) prediction accuracy are represented by white and black colours, respectively. The recognition of the current gait period, from the CNN, is shown in orange colour. For example, when the current gait period during level-ground walking is recognised as period 1 (initial contact), the next most probable gait period is period 2 (loading response) with a prediction accuracy of 99.5% (see plot A). Prediction accuracy of gait periods for level-ground walking (LGW), ramp ascent (RA) and ramp descent (RD) is presented in confusion matrices (A), (B) and (C), respectively.

TABLE I

COMPARISON OF STATE-OF-THE-ART METHODS FOR RECOGNITION OF WALKING ACTIVITIES AND PREDICTION OF GAIT PERIODS

Method	Activity	# Sensors	Recognition activity accuracy (%)	Recognition gait period accuracy (%)	Prediction gait period accuracy (%)
Log-sum distance [25]	Level walking, ramps, sitting	9	99.0	-	-
ANN [26]	Level walking	32	98.78	-	-
LDA + DBN [27]	Level walking, ramps, stair	13	99.5	-	-
GMM [28]	Level walking, standing, sitting	4	100	-	-
SVM [29]	Level walking, ramps	9	99	97	-
DBN [30]	Level walking, ramps, stair	13	98	95.25	-
CNN + first-order MC	Level walking, ramps	3	100	98.32	98.23

IV. CONCLUSION

In this work we presented a strategy, composed of a CNN and first-order MC, for recognition of walking activities and prediction of gait periods using data from wearable sensors. The CNN was implemented for recognition of walking activities (level-ground walking, ramp ascent and descent) and gait periods (initial contact, loading response, mid-stance, terminal stance, pre-swing, initial swing, mid-swing and terminal swing), achieving mean accuracies of 100%, and 98.32%, respectively. The first-order MC was developed to predict the next probable or expected gait period during the gait cycle. This temporal model achieved mean accuracies of 99.78%, 97.56% and 97.35% for prediction during level-ground walking, ramp ascent and descent, respectively. All the experiments, for validation of the proposed method, employed real data collected from three wearable sensors attached to the thigh, shank and foot of participants while performing walking activities. The results showed that our method is able to identify the state of the human body and estimate the next expected event during the walking activity. Overall, the recognition and predictive functionalities, offered by the proposed strategy, are essential for control of intelligent wearable devices capable to provide safe and reliable assistance to humans in ADLs.

REFERENCES

- [1] S. W. Brose, D. J. Weber, B. A. Salatin, G. G. Grindle, H. Wang, J. J. Vazquez, and R. A. Cooper, "The role of assistive robotics in the lives of persons with disability," *American Journal of Physical Medicine & Rehabilitation*, vol. 89, no. 6, pp. 509–521, 2010.
- [2] H. Zhou and H. Hu, "Human motion tracking for rehabilitation—a survey," *Biomedical Signal Processing and Control*, vol. 3, no. 1, pp. 1–18, 2008.
- [3] U. Martinez-Hernandez, I. Mahmood, and A. A. Dehghani-Sanij, "Simultaneous bayesian recognition of locomotion and gait phases with wearable sensors," *IEEE Sensors Journal*, vol. 18, no. 3, pp. 1282–1290, Feb 2018.
- [4] U. Martinez-Hernandez and A. A. Dehghani-Sanij, "Probabilistic identification of sit-to-stand and stand-to-sit with a wearable sensor," *Pattern Recognition Letters*, 2018. [Online]. Available: <https://doi.org/10.1016/j.patrec.2018.03.020>
- [5] C. Kirtley, *Clinical gait analysis: theory and practice*. Elsevier Health Sciences, 2006.
- [6] U. Martinez-Hernandez, L. W. Boorman, and T. J. Prescott, "Multisensory wearable interface for immersion and telepresence in robotics," *IEEE Sensors Journal*, vol. 17, no. 8, pp. 2534–2541, 2017.
- [7] S. Patel, H. Park, P. Bonato, L. Chan, and M. Rodgers, "A review of wearable sensors and systems with application in rehabilitation," *Journal of neuroengineering and rehabilitation*, vol. 9, no. 1, 2012.

- [8] Y. Mengüç, Y.-L. Park, H. Pei, D. Vogt, P. M. Aubin, E. Winchell, L. Fluke, L. Stirling, R. J. Wood, and C. J. Walsh, "Wearable soft sensing suit for human gait measurement," *The International Journal of Robotics Research*, vol. 33, no. 14, pp. 1748–1764, 2014.
- [9] U. Martinez-Hernandez and A. A. Dehghani-Sanij, "Adaptive bayesian inference system for recognition of walking activities and prediction of gait events using wearable sensors," *Neural Networks*, vol. 102, pp. 107 – 119, 2018.
- [10] A. Young, T. Kuiken, and L. Hargrove, "Analysis of using emg and mechanical sensors to enhance intent recognition in powered lower limb prostheses," *Journal of neural engineering*, vol. 11, no. 5, 2014.
- [11] Y. LeCun, Y. Bengio, and G. Hinton, "Deep learning," *Nature*, vol. 521, no. 7553, pp. 436–444, 2015.
- [12] J. Schmidhuber, "Deep learning in neural networks: An overview," *Neural networks*, vol. 61, pp. 85–117, 2015.
- [13] C. Bishop, *Pattern Recognition and Machine Learning*, ser. Information Science and Statistics. Springer, 2006.
- [14] T. V. Duong, H. H. Bui, D. Q. Phung, and S. Venkatesh, "Activity recognition and abnormality detection with the switching hidden semi-markov model," in *Computer Vision and Pattern Recognition, 2005. CVPR 2005*, vol. 1. IEEE, 2005, pp. 838–845.
- [15] U. Martinez-Hernandez, T. J. Dodd, and T. J. Prescott, "Feeling the shape: Active exploration behaviors for object recognition with a robotic hand," *IEEE Transactions on Systems, Man, and Cybernetics: Systems*, vol. PP, no. 99, pp. 1–10, 2017. [Online]. Available: <http://doi.org/10.1109/TSMC.2017.2732952>
- [16] S. Thrun, W. Burgard, and D. Fox, *Probabilistic robotics*. MIT, 2005.
- [17] R. A. Brooks, "A robust layered control system for a mobile robot," *Journal of Robotics and Automation*, vol. 2, no. 1, pp. 14–23, 1986.
- [18] O. Abdel-Hamid, A.-r. Mohamed, H. Jiang, L. Deng, G. Penn, and D. Yu, "Convolutional neural networks for speech recognition," *IEEE/ACM Transactions on audio, speech, and language processing*, vol. 22, no. 10, pp. 1533–1545, 2014.
- [19] A. Krizhevsky, I. Sutskever, and G. E. Hinton, "Imagenet classification with deep convolutional neural networks," in *Advances in neural information processing systems*, 2012, pp. 1097–1105.
- [20] A. Rubio-Solis and G. Panoutsos, "Interval type-2 radial basis function neural network: a modeling framework," *IEEE Transactions on Fuzzy Systems*, vol. 23, no. 2, pp. 457–473, 2015.
- [21] U. Martinez-Hernandez, T. J. Dodd, M. H. Evans, T. J. Prescott, and N. F. Lepora, "Active sensorimotor control for tactile exploration," *Robotics and Autonomous Systems*, vol. 87, pp. 15–27, 2017.
- [22] J. Ying, T. Kirubarajan, K. R. Pattipati, and A. Patterson-Hine, "A hidden markov model-based algorithm for fault diagnosis with partial and imperfect tests," *IEEE Transactions on Systems, Man, and Cybernetics, Part C*, vol. 30, no. 4, pp. 463–473, 2000.
- [23] A. Rubio-Solis, U. Martinez-Hernandez, and G. Panoutsos, "Evolutionary extreme learning machine for the interval type-2 radial basis function neural network: A fuzzy modelling approach," in *World Congress on Computational Intelligence*. IEEE, 2018 (in press).
- [24] H. C. Cho and S. M. Fadali, "Online estimation of dynamic bayesian network parameter," in *Neural Networks, 2006. IJCNN'06. International Joint Conference on*. IEEE, 2006, pp. 3363–3370.
- [25] F. Sikder and D. Sarkar, "Log-sum distance measures and its application to human-activity monitoring and recognition using data from motion sensors," *IEEE Sensors Journal*, 2017.
- [26] K. Zhang, M. Sun, D. K. Lester, F. X. Pi-Sunyer, C. N. Boozer, and R. W. Longman, "Assessment of human locomotion by using an insole measurement system and artificial neural networks," *Journal of Biomechanics*, vol. 38, no. 11, pp. 2276–2287, 2005.
- [27] A. J. Young and L. J. Hargrove, "A classification method for user-independent intent recognition for transfemoral amputees using powered lower limb prostheses," *IEEE Transactions on Neural Systems and Rehabilitation Engineering*, vol. 24, no. 2, pp. 217–225, 2016.
- [28] H. A. Varol, F. Sup, and M. Goldfarb, "Multiclass real-time intent recognition of a powered lower limb prosthesis," *Biomedical Engineering, IEEE Transactions on*, vol. 57, no. 3, pp. 542–551, 2010.
- [29] H. Huang, F. Zhang, L. J. Hargrove, Z. Dou, D. R. Rogers, and K. B. Englehart, "Continuous locomotion-mode identification for prosthetic legs based on neuromuscular–mechanical fusion," *Biomedical Engineering, IEEE Transactions on*, vol. 58, no. 10, pp. 2867–2875, 2011.
- [30] A. J. Young, A. M. Simon, N. P. Fey, and L. J. Hargrove, "Intent recognition in a powered lower limb prosthesis using time history information," *Annals of biomedical engineering*, vol. 42, no. 3, pp. 631–641, 2014.