



This is a repository copy of *A feasibility investigation of speciation by Fe K-edge XANES using a laboratory X-ray absorption spectrometer.*

White Rose Research Online URL for this paper:

<https://eprints.whiterose.ac.uk/163080/>

Version: Accepted Version

Article:

Mottram, L.M., Cafferkey, S., Mason, A.R. et al. (5 more authors) (2020) A feasibility investigation of speciation by Fe K-edge XANES using a laboratory X-ray absorption spectrometer. *Journal of Geosciences*, 65 (1). pp. 27-35. ISSN 1802-6222

<https://doi.org/10.3190/jgeosci.299>

© 2020 Czech Geological Society. This is an author-produced version of a paper subsequently published in *Journal of GEOsciences*. Uploaded with permission from the copyright holder.

Reuse

Items deposited in White Rose Research Online are protected by copyright, with all rights reserved unless indicated otherwise. They may be downloaded and/or printed for private study, or other acts as permitted by national copyright laws. The publisher or other rights holders may allow further reproduction and re-use of the full text version. This is indicated by the licence information on the White Rose Research Online record for the item.

Takedown

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing eprints@whiterose.ac.uk including the URL of the record and the reason for the withdrawal request.



eprints@whiterose.ac.uk
<https://eprints.whiterose.ac.uk/>

Original paper

**A feasibility investigation of speciation by Fe K edge XANES using a
laboratory X-ray absorption spectrometer**

Lucy M. Mottram¹, Samuel Cafferkey,¹ Amber R. Mason, Tom Oulton,¹ Shi Kuan Sun,¹

Daniel J. Bailey,¹ Martin C. Stennett¹, and Neil C. Hyatt^{1*}

*1 Department of Materials Science and Engineering, The University of Sheffield,
Mappin Street, Sheffield, S1 3JD, UK;*

n.c.hyatt@sheffield.ac.uk

** Corresponding author*

Keywords: XANES, X-ray Absorption Spectroscopy, iron, speciation, laboratory.

Running title: Speciation by laboratory Fe K-edge XANES

Abstract

We demonstrate effective speciation of Fe in model compounds from analysis of the weak pre-edge features in Fe K-edge XANES spectra, with a commercially available laboratory X-ray spectrometer, using a spherically bent crystal analyser, and a low power X-ray tube, in Rowland circle geometry. Direct comparison with XANES data acquired from a third generation synchrotron bending magnet beamline, using the same specimens, validated quantitative agreement in determination of the total integrated intensity and centroid position of the pre-edge feature, which are a probe of the electronic configuration and symmetry of the absorber atom, and hence oxidation state and co-ordination number. This work opens the door to rapid and routine speciation studies of Fe by laboratory XANES, even for materials with relatively dilute absorber concentration of only a few mol%.

1. Introduction

The redox chemistry of iron is of fundamental importance in Earth science and plays a crucial role in geochemical and biogeochemical processes (Taylor and Konhauser 2011). Iron is so far known to adopt formal oxidation states from Fe^{2-} to Fe^{6+} , although the most common oxidation states are ferrous Fe^{2+} and ferric Fe^{3+} (Greenwood and Earnshaw 1997). Redox transformations involving Fe^{2+} and Fe^{3+} are of critical importance in geological, environmental, biological and material processes, and, for example, the $\text{Fe}^{2+} / \text{Fe}^{3+}$ ratio is commonly exploited to constrain the conditions of mineral and glass formation (Wood and Virgo 1989; Taylor and Konhauser 2011; Joseph et al. 2017). X-ray absorption spectroscopy (XAS) has proven a powerful tool for the determination of Fe speciation in minerals and materials (Waychunas et al. 1983; Bajt et al. 1994; Galois et al. 2001; Petit et al. 2001; Wilke et al. 2001; Berry et al. 2003; Joseph et al. 2017), however, routine application is inhibited by the requirement to access XAS beamlines at synchrotron radiation facilities, which is highly competitive, time limited, and not immediate. The weak pre-edge features in the Fe K-edge X-ray Absorption Near Edge Structure (XANES), located ca. 15 - 20 eV below the edge step, have been shown to be a particularly sensitive probe of Fe speciation (Waychunas et al. 1983; Bajt et al. 1994; Galois et al. 2001; Petit et al. 2001; Wilke et al. 2001; Berry et al. 2003; Joseph et al. 2017). These features are associated with 1s – 3d (quadrupole) and/or 1s – 4p (dipole) electronic transitions in the Fe absorber atom and, therefore, are sensitive to both the electronic configuration and symmetry, from which oxidation state and co-ordination number are inferred.

Wilke *et al.* developed a systematic methodology to extract the normalised pre-edge features from Fe K-edge XANES data and determination of the centroid energy position and total integrated intensity, which was effectively correlated with Fe oxidation state and co-ordination number (Petit et al. 2001; Wilke et al. 2001). This methodology utilised high

resolution XANES data from mineral reference compounds, primarily acquired using the undulator beamline ID26 with a Si (220) double crystal monochromator, at the European Synchrotron Radiation Facility. This methodology has subsequently been widely applied (685 citations up to the end of 2019 (Wilke et al. 2001)).

In recent years, a renaissance in laboratory instrumentation for X-ray absorption and emission spectroscopy, has been driven by exploitation of Spherically Bent Crystal Analysers (SBCAs) in a Rowland circle geometry or bent cylindrical monochromators in von Hamos geometry (Seidler et al. 2014, 2016; Schlesiger et al. 2015; Mortensen et al. 2016; Nemeth et al. 2016; Holden et al. 2017; Malzer et al. 2018; Jahrman et al. 2019; Blachucki et al. 2019; Honkanen et al. 2019; Jahrman et al. 2019; Zeeshan et al. 2019; Mottram et al. 2020). In principle, such instrumentation may allow good quality X-ray absorption or emission spectroscopy to be *routinely* acquired from materials with moderately dilute to concentrated absorbers in a matter of hours, without recourse to a synchrotron light source. Here, we report the results of a preliminary comparative investigation of Fe speciation by analysis of weak pre-edge features in Fe K-edge X-ray Absorption Near Edge Structure (XANES) using a commercially available laboratory spectrometer based on the design of Seidler *et al.*, which is also capable of acquisition of the full Extended X-ray Absorption Fine Structure (EXAFS) in favourable circumstances (Seidler et al. 2014, 2016; Mortensen et al. 2016; Jahrman et al. 2019). The spectrometer arrangement utilises SBCAs in a 1m Rowland circle geometry, Fig. 1 and Fig. 2, in which energy scanning is achieved through symmetrical movement of detector and source. Linear translation stages are used to increment Bragg angle steps, with the alignment of source, SBCA and detector maintained by steering bars. The spectrometer operates close to back scattering geometry to maximise resolution and thus requires a different SBCA to scan several hundred eV. In our set up, the high efficiency of the SBCAs enables the use of a relatively inexpensive, low power, air cooled, X-ray source (100 W), which is sufficient for

transmission mode investigation of moderately dilute absorbers in a favourable matrix, with a data collection time of several hours (it is also possible to utilise a fixed X-ray source of 1.5kW with suitable modification of the optical arrangement, as highlighted by Honkanen et al. 2019) With robust initial SBCA alignment (Mortensen et al. 2017), change over and alignment of SBCAs is straightforward and can be achieved in 20 minutes or less. In the following, we first compare the resolution performance of this laboratory spectrometer in comparison with a synchrotron bending magnet beamline at a third generation synchrotron source. Using the well established methodology of Wilke *et al.* (Petit et al. 2001; Wilke et al. 2001), we then demonstrate that laboratory XANES data from reference compounds can be analysed to accurately infer Fe speciation from the weak pre-edge features, even in the case of a relatively dilute Fe concentration of a few mol %.

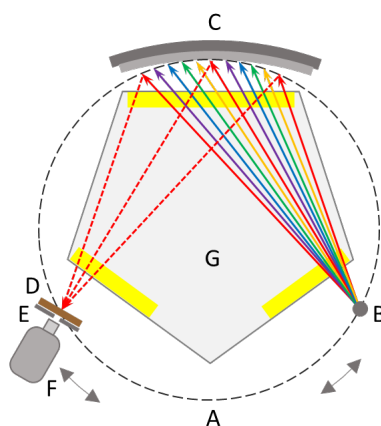


Fig. 1 Schematic representation of Rowland circle geometry for laboratory transmission X-ray Absorption Spectroscopy, as described in the text, showing: Rowland circle (A), broadband low power X-ray source (B); spherically bent crystal analyser (C); sample (D) and slit (E) arrangement; silicon drift detector (F); and helium filled beam path with kapton windows (G).



Fig. 2 Photograph of EasyXAFS XES100 spectrometer arrangement shown in Fig. 1, with helium filled beam path removed, to show linear translation stages and steering bars used to maintain alignment of X-ray source (A), spherically bent crystal analyser (B); and sample, slit and detector assembly (C).

2. Materials and Methods

2.1. Materials

The materials investigated in this study are summarised in Tab. 1. $\text{NaFeSi}_2\text{O}_6$ and FePO_4 are characterised by Fe^{3+} , co-ordinated by oxygen in an octahedral and tetrahedral co-ordination, respectively (Arnold 1986; Baum et al. 1988). Fe_2SiO_4 and $\text{Fe}_{1.5}\text{Mg}_{0.5}\text{Al}_{9.1}\text{Si}_{3.9}(\text{OH})_2$ are characterised by Fe^{2+} , co-ordinated by oxygen in an octahedral and tetrahedral co-ordination, respectively (Smyth 1975; Hawthorne et al. 1993). Polycrystalline FePO_4 and Fe_2SiO_4 were, respectively, synthesised by: solid state reaction of Fe_2O_3 and $\text{NH}_4\text{H}_2\text{PO}_4$ at 900 °C in air for 16 h; and solid state reaction of stoichiometric quantities of Fe, Fe_2O_3 and SiO_2 at 750 °C for

48 h in a sealed, evacuated, quartz tube. Mineral specimens of agerine - $\text{NaFeSi}_2\text{O}_6$ (Langesund Fjord, Norway), and staurolite – $\text{Fe}_{1.5}\text{Mg}_{0.5}\text{Al}_{9.1}\text{Si}_{3.9}(\text{OH})_2$ (Georgia, USA), were provided from our own collection. All materials were confirmed to be single phase by powder X-ray diffraction. The expected Fe speciation was verified by ^{57}Fe Mossbauer analysis.

Material	Fe oxidation state	CN	Fe Concentration (mol%)	Lab data collection time (h)
$\text{NaFeSi}_2\text{O}_6$ <i>Agerine: Langesund Fjord (Norway)</i>	3+	6 (O_h)	10.0	6
FePO_4 <i>Synthetic</i>	3+	4 (T_d)	16.7	5
Fe_2SiO_4 <i>Synthetic</i>	2+	6 (O_h)	28.6	4
$\text{Fe}_{1.5}\text{Mg}_{0.5}\text{Al}_{9.1}\text{Si}_{3.9}(\text{OH})_2$ <i>Staurolite: Georgia (USA)</i>	2+	4 (T_d)	3.7	8

Tab. 1 Materials analysed in this study, summarising Fe oxidation state, co-ordination number by oxygen (and symmetry), Fe concentration, and data collection time.

2.2. X-ray absorption spectroscopy

Fe K-edge XANES data were acquired in transmission mode using a commercially available laboratory spectrometer and the DUBBLE beamline, BM 26, of the European Synchrotron Radiation Facility.

The laboratory spectrometer, based on the design of Seidler *et al.* (Seidler *et al.* 2014, 2016; Mortensen *et al.* 2016; Jahrman *et al.* 2019), was an EasyXAFS XES100 system, equipped with an air cooled X-ray tube operating at 25 kV and 4 mA, with a Hitachi Vortex Silicon Drift Detector (SDD). The spectrometer was configured with a Ge (620) SBCA to scan the energy range 6970 – 7340 eV, with a step size of 0.25 – 1.00 eV and constant count time of 4s / point in the XANES region (total scan time 30 min for 0.25 eV step size). The energy resolution of the SDD is ca. 140 eV, enabling rejection of the harmonic content of the incident beam and background scatter. A He flight path was used to minimise air scatter and

absorption. Transmission data were acquired with ($I_t(E)$) and without the sample ($I_0(E)$), using the same scan parameters. The Ge (620) monochromator was aligned using the clock angle procedure of Mortensen and Seidler, to account for the crystal miscut (Mortensen et al. 2017).

The DUBBLE beamline is situated on a bending magnet and was configured with a Si (111) channel cut monochromator and Si mirror for harmonic rejection (Borsboom et al. 1988). Incident and transmitted beam intensities were measured using ionization chambers, filled with mixtures of He and N₂, operated in a stable region of their I/V curve. For synchrotron data, a step size of 0.25 eV was used in the XANES region with a count time of 1s / point. Samples were prepared from finely ground specimens dispersed in 70 mg of polyethylene glycol, pressed into 13 mm diameter pellets, to achieve a thickness of one absorption length. Data reduction and analysis was performed using the programs Athena and Hephaestus (Ravel et al. 2005). Calibration of the energy scale was achieved by reference to a 5 μm Fe foil (Goodfellow Cambridge Ltd.), for which the first peak in the derivative spectrum was set to 7112.00 eV, as defined by Bearden and Burr for the Fe K absorption edge (Bearden et al. 1967). For laboratory XANES data, Fe foil data were acquired using the same methods as for the sample materials. The Bragg angle of $\theta = 77.7084^\circ$, corresponding to the first peak of the derivative spectrum was set equivalent to 7112.00 eV, enabling the energy scale to be calibrated according to:

$$E_c = \frac{E_m \sin(\theta)}{\sin(\theta + \Delta\theta)}$$

where, E_m is the measured energy, E_c the calibrated energy, $\Delta\theta$ is the difference between the Bragg angle corresponding to E_c and E_m .

For synchrotron XANES data, an Fe foil was measured simultaneously with the samples, and the energy scale calibrated using the alignment tool in the Athena program (Ravel et al.

2005). Extraction and analysis of the pre-edge feature in Fe K-edge XANES data was achieved using Microsoft Excel software, to first fit a spline function to model and subtract the contribution of the edge step. The pre-edge envelope was then deconvoluted by fitting Gaussian components using a linear least squares refinement to optimise the normalised height, full width at half height, and energy position, so as to minimise the difference between the observed and calculated envelope determined from the sum of the fitted Gaussian components. Fitting initially utilised two Gaussian components with the significance of a third component tested by inspection of the improvement in goodness of fit. The total integrated intensity and centroid energy of the pre-edge feature were determined, respectively, from the sum of the integrated intensities and intensity weighted average energy position of the Gaussian components. The same initial parameters were used for all data sets, and several sets of different initial parameters trialled, to ensure that convergence did not arise in a local minimum. This approach is a simplification of that applied by Wilke *et al.*, which employed pseudo-Voigt components (Petit *et al.* 2001; Wilke *et al.* 2001).

3. Results

3.1. Spectrometer performance at Fe K-edge

The robustness of the laboratory spectrometer and resolution at the Fe K-edge was investigated by acquisition and analysis of XANES data from an Fe foil. Fig. 3 shows the result of a merging 10 individual XANES scans (0.25 eV resolution, black line), between each individual scan, the sample carousel was removed and the Fe foil unmounted. Data were background subtracted and normalised prior to merging, but were not aligned. The resulting standard deviation in the merged data (red line) shown in Fig. 3, attests to robustness of the spectrometer alignment and scan to scan reproducibility. Next, as shown in Fig. 4, laboratory data were acquired at step sizes of 0.25, 0.50, 0.75 and 1.00 eV in the XANES region (points)

and compared with synchrotron data from the DUBBLE beamline acquired at 0.25 eV step size (solid line), as the first derivative to amplify the XANES features. Comparison of these spectra shows that a step size of 0.5 eV accurately approximates the synchrotron data, but a step size of 0.75 eV or greater does not fully resolve features apparent in the synchrotron data. The resolution of our laboratory data are therefore comparable with that achievable with a Si (111) monochromator on a bending magnet beamline at a third generation synchrotron source, providing confidence in the characterisation of weak pre-edge features. Note that the core-hole life time is estimated to impose a limiting resolution of 1.25 eV at the Fe K-edge (Krause et al. 1979), which dominates the resolution of both our laboratory and synchrotron data. For the purpose of head to head comparison a step size of 0.25 eV was maintained for acquisition of XANES data from Fe reference compounds.

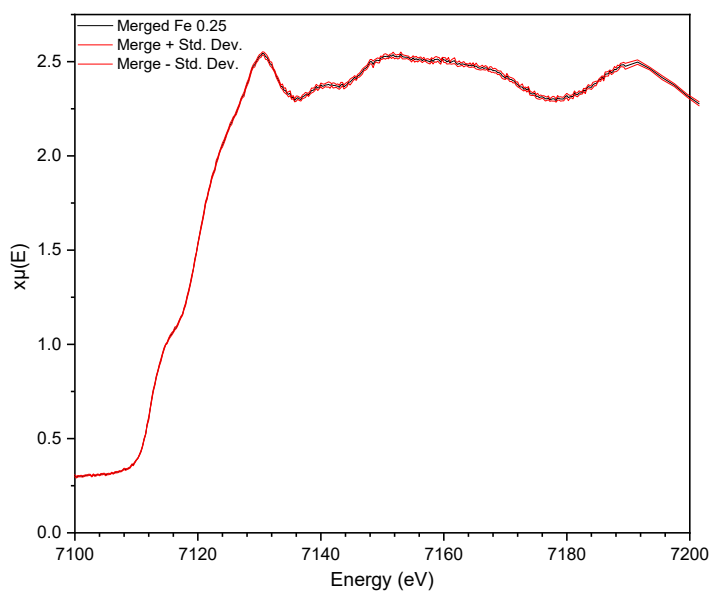


Fig. 3 – Merge of 10 independent XANES data sets from Fe foil (0.25 eV resolution, black line) with standard deviation (red line).

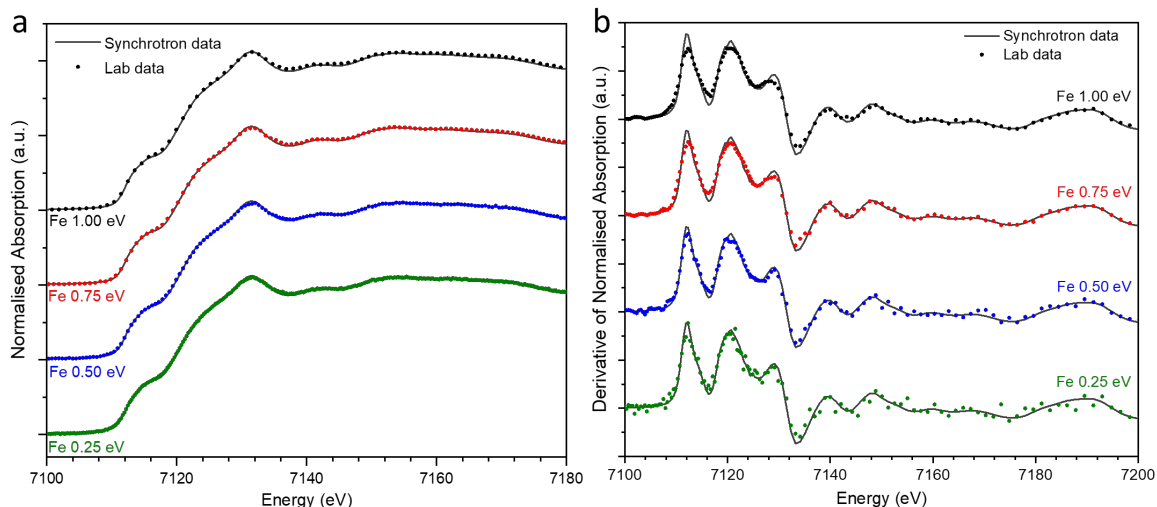


Fig 4a – Comparison of synchrotron (0.25 eV resolution, black line) and laboratory (0.25 – 1.00 eV resolution, points) acquired XANES data; **b** - Comparison of first derivative of synchrotron (0.25 eV resolution, black line) and laboratory (0.25 – 1.00 eV resolution, points) acquired XANES data, to emphasise correspondence of features.

3.2. Laboratory and synchrotron Fe K-edge XANES of model compounds

Fig. 5 compares the laboratory and synchrotron Fe K-edge XANES data acquired from the reference compounds in Tab. 1. Overall, the observed chemical shift and XANES features are in excellent agreement between the data sets, when the synchrotron data are convoluted by a Lorentzian function of 0.75 eV full width at half maximum (FWHM). For the staurolite data in particular, which presents relatively sharp features in the region of the white line, this convolution greatly improves the agreement between synchrotron and laboratory data. We also corrected laboratory data for the “leakage” effect, which arises from contamination of I_0 and I_t by photons arising from the low energy tail of the monochromator function, harmonics and scattering (I_{lk}) (Stern et al. 1981). Consequently, $\mu = \ln(I_0 - I_{0,lk}) / (I_t - I_{t,lk})$, and thus μ no longer strictly depends on I_0 and I_t . In simple terms, the distortion arises because, at the white line, where μ is a maximum, I_{lk} makes a non-negligible contribution to the measured I_t ,

which is small because of the dilute concentration in a relatively absorbing matrix: thus, the measured absorption is less than the true absorption. In the present investigation, this correction had marginal impact on the laboratory XANES data.

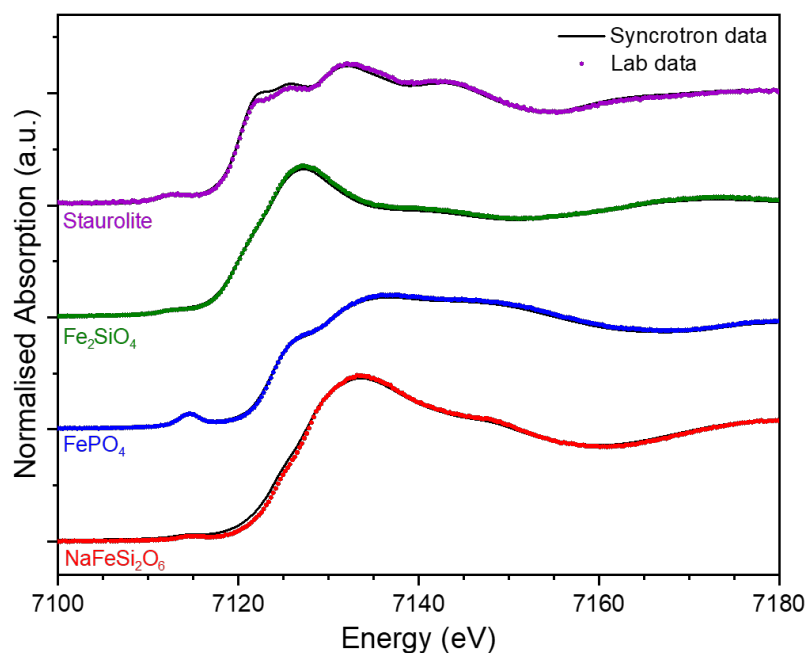


Fig. 5 Comparison of normalised transmission mode Fe K-edge XANES spectra from reference compounds $\text{NaFeSi}_2\text{O}_6$, FePO_4 , Fe_2SiO_4 , and staurolite – $\text{Fe}_{1.5}\text{Mg}_{0.5}\text{Al}_{9.1}\text{Si}_{3.9}(\text{OH})_2$, (prepared to $\mu\text{x} = 1$), acquired using laboratory XAS spectrometer (points) and DUBBLE beamline (solid line); synchrotron data were broadened by a Lorentzian function of 0.75 eV FWHM.

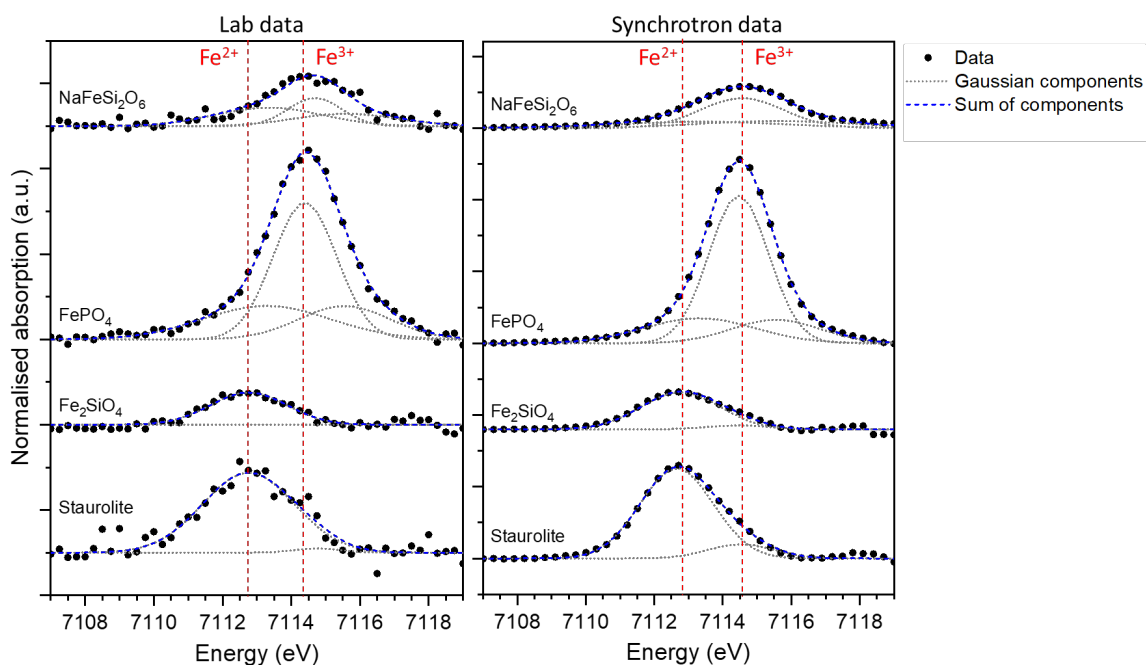


Fig. 6 Normalised pre-edge spectra at Fe K edge (points) from reference compounds NaFeSi₂O₆, FePO₄, Fe₂SiO₄, and Fe_{1.5}Mg_{0.5}Al_{9.1}Si_{3.9}(OH)₂, acquired using laboratory XAS spectrometer and DUBBLE beamline, showing fitted Gaussian components (grey dotted line) and their summation envelope (blue dotted line).

Fig. 7 and Tab. 2 compare the extracted pre-edge features from laboratory and synchrotron XANES data and the modelled envelope of the Gaussian components (here the synchrotron data are not convoluted by Lorentzian broadening). For each material, the pre-edge features of the laboratory and synchrotron XANES data were adequately modelled using the same number of Gaussian components (either two or three). Although the laboratory data clearly demonstrate more scatter in comparison to the synchrotron data, as expected due to lower signal to noise ratio, the correspondence between the data sets is remarkable. The centroid energy of the pre-edge features of Fe²⁺ and Fe³⁺ species are clearly distinguished at 7112.9 ± 0.1 eV and 7114.5 ± 0.1 eV respectively, in both the laboratory and synchrotron data. For each Fe species, the measured normalised intensity of the pre-edge feature is also in excellent

agreement between laboratory and synchrotron data sets. As expected, the pre-edge features of the tetrahedral Fe species present in FePO_4 and $\text{Fe}_{1.5}\text{Mg}_{0.5}\text{Al}_{9.1}\text{Si}_{13.9}(\text{OH})_2$, have considerably greater intensity than those of the octahedral species present in $\text{NaFeSi}_2\text{O}_6$ and Fe_2SiO_4 . As noted above, and discussed below, the pre-edge features are primarily associated with 1s – 3d quadrupole transitions, which are only weakly allowed for octahedral Fe since the initial and final states are centrosymmetric. In the non-centrosymmetric tetrahedral environments, the transition probability is enhanced due to admixture of unoccupied 4p orbitals in the final state.

Material	Gaussian 1		Gaussian 2		Gaussian 3		Centroid Energy (eV)	Total integrated intensity (a.u.)
	Energy (eV)	Intensity (a.u.)	Energy (eV)	Intensity (a.u.)	Energy (eV)	Intensity (a.u.)		
$\text{NaFe}_2\text{SiO}_6$ <i>Agerine: Langesund Fjord (Norway)</i>	7113.3 7113.4	0.042 0.027	7114.7 7114.6	0.032 0.063	7115.6 7115.6	0.027 0.028	7114.5 7114.6	0.102 0.117
FePO_4 <i>Synthetic</i>	7113.3 7113.3	0.091 0.071	7114.5 7114.5	0.186 0.225	7115.4 7115.5	0.065 0.053	7114.4 7114.4	0.343 0.349
Fe_2SiO_4 <i>Synthetic</i>	7112.7 7112.8	0.063 0.075	7115.8 7114.5	0.002 0.006	-	-	7112.8 7112.9	0.063 0.081
$\text{Fe}_{1.5}\text{Mg}_{0.5}\text{Al}_{9.1}\text{Si}_{13.9}(\text{OH})_2$ <i>Staurolite: Georgia (USA)</i>	7112.8 7112.7	0.157 0.169	7114.8 7114.5	0.004 0.024	-	-	7112.9 7112.9	0.161 0.192

Tab. 2 Integrated intensity and centroid energy for Gaussian components fitted to pre-edge features, and intensity weighted centroid position and total integrated intensity of fitted pre-edge envelope. Values in bold type are derived from laboratory data; values in normal type are derived from synchrotron data.

Fig. 7 compares the total integrated intensity and centroid energy of modelled pre-edge features extracted from our laboratory and synchrotron XANES data, and the synchrotron data reported by Wilke *et al.* (Petit *et al.* 2001; Wilke *et al.* 2001). To construct this plot, the data of Wilke *et al.* (calibrated to $E_0 = 7111.08$ eV), were shifted by +0.92 eV, consistent with our absolute energy scale. Fig. 7 shows that Fe speciation is clearly differentiated according to the total integrated intensity and centroid position of the pre-edge feature. The data points determined from laboratory and synchrotron data, acquired from identical materials, and

corresponding data points acquired by Wilke *et al.* on their materials, are seen to be in good overall agreement (solid points in Fig. 7). A systematic difference of ca. 0.25 eV is apparent between the pre-edge centroid energy determined from our laboratory and synchrotron data. This is of the order of the measurement step size and, therefore, likely arises from a small difference in calibration of the absolute energy scale (see also Tab. 2). The spread in determined total integrated intensities is approximately 15 – 20 % relative, with the laboratory determination systematically lower than our synchrotron determination. In the case of our laboratory data, the contribution of intensity in the tails of the pre-edge features is underestimated by the fitted Gaussian components, due to the lower signal to noise. Nevertheless, it is clear that both our laboratory and synchrotron data fall within the known Fe²⁺ and Fe³⁺ speciation fields, as shown by Fig. 7. Some scatter is apparent between our synchrotron data points and those of Wilke *et al.*, for the same nominal materials, however, given that the samples, experimental set ups, and data analysis methods are not identical, we believe the overall agreement between the studies to validate the determination of Fe speciation by laboratory XANES data.

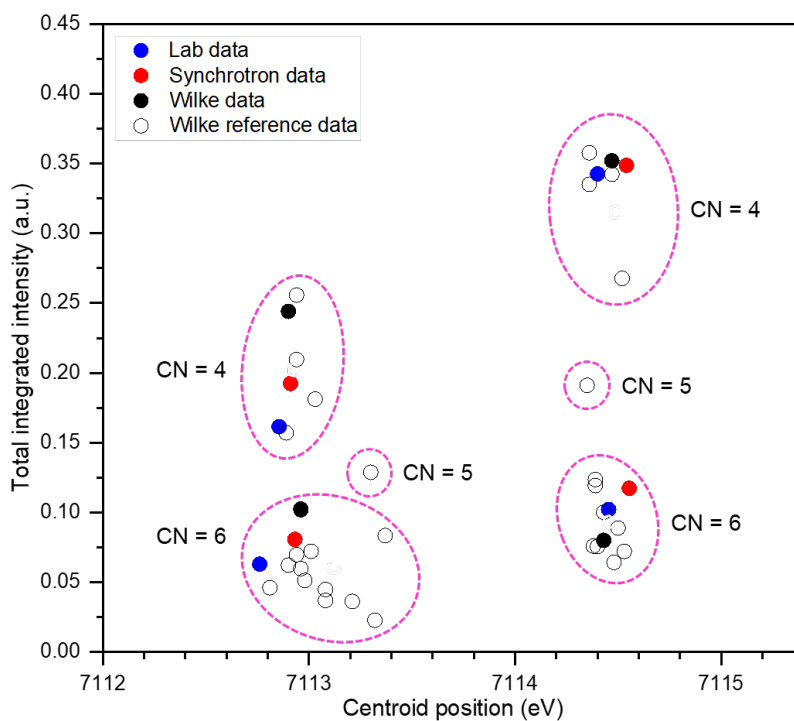


Fig. 7 Speciation field diagram, based on total integrated intensity and centroid energy of pre-edge feature of Fe K-edge XANES data. Data points derived from analysis of our laboratory and synchrotron data are shown as solid blue and red circles, respectively, equivalent data points from Wilke *et al.* (Wilke *et al.* 2001) shown as solid black circles. Other reference data from Wilke *et al.*, shown as open black circles. Note data from Wilke *et al.*, are shifted by +0.92 eV consistent with our absolute energy scale as described in the text.

4. Discussion

The data presented in Fig. 5-7 show that good quality XANES data may be acquired in a matter of hours from compounds with moderately dilute to high Fe concentration, using a commercially available spectrometer, enabling routine speciation of Fe in the laboratory.

Optimisation of the data acquisition strategy may yield efficiency gains for routine application. Good signal to noise, and a sufficiently small step size, are essential in the region

of the pre-edge and rising absorption edge, to enable accurate isolation of the pre-edge feature with optimal resolution. However, outside of this range, the density of data points used in this study could potentially be reduced by a factor of 2-4, without impacting on accuracy or precision of the pre-edge analysis, for high throughput routine analysis.

The weak pre-edge features observed in Fe K-edge XANES data are associated primarily with $1s - 3d$ (quadrupole) and $1s - 4p$ (dipole) electronic transitions (Waychunas et al. 1983; Bajt et al. 1994; Galois et al. 2001; Petit et al. 2001; Wilke et al. 2001; Berry et al. 2003; Joseph et al. 2017). The pre-edge envelope is typically comprised of two or more components which arise from transitions to $3d$ final states which are non-degenerate as a result of the crystal field imposed by the local environment of the Fe absorber. Thus, crystal field theory predicts two and three allowed transitions, respectively, for Fe^{2+} ($[Ar]3d^6$ *hs*) in tetrahedral and octahedral field, whereas, two allowed transitions are predicted for Fe^{3+} ($[Ar]3d^5$ *hs*) in tetrahedral and octahedral crystal fields respectively (*hs*: high spin) (Westre et al. 1997; Baker et al. 2017). Additional contributions to the pre-edge feature have been reported for some distorted Fe^{3+} octahedral environments (such as in Fe_2O_3) which are attributed to admixture of $4p$ states and availability of unoccupied delocalised states (Dräger et al. 1988; de Groot et al. 2009). In this investigation, and others (Petit et al. 2001; Wilke et al. 2001), deconvolution of the pre-edge feature requires fewer components than the number of allowed transitions, due to a combination of the magnitude of the crystal field splitting, distortion from ideal coordination geometry, limited spectral resolution compared to the core-hole life time, and other factors. Nevertheless, as demonstrated by Fig. 7, the total integrated intensity and centroid energy of the pre-edge feature can be accurately estimated by fitting of Gaussian or pseudo-Voigt functions, and is correlated with the electronic configuration and symmetry of the absorber and hence oxidation state and co-ordination number.

The chemical shift between the centroid energy of Fe²⁺ and Fe³⁺ species determined in this investigation was 1.6 ± 0.1 eV for both laboratory and synchrotron XANES data, in excellent agreement with the value of 1.4 ± 0.1 eV determined by Wilke *et al.* (Wilke et al. 2001). Our laboratory and synchrotron data can be brought into approximate co-incidence in Fig. 6, by a shift of approximately 0.25 eV in energy and 0.025 a.u. in total integrated intensity, which implies that the differences between our measurements arise principally from systematic error. Consequently, it is preferable that a comprehensive reference data set (including reference mixtures) be acquired to define the speciation fields (and their joins), for each specific instrument (whether laboratory or synchrotron) to enable the most accurate speciation. This will form the objective of the next phase of this study.

As pointed out by Wilke *et al.* (Wilke et al. 2001), Fe speciation can be determined unambiguously in the case of a single dominant species or a binary mixture, from analysis of the pre-edge feature in Fe K-edge XANES. However, unique determination of more complex mixtures, or the presence of 5 co-ordinate Fe, is more difficult to ascertain, although the location of extracted data in the structure field map of Fig. 7 at least provides some insight into the likely component species. For such cases, modelling of the extended X-ray absorption fine structure, additional ⁵⁷Fe Mossbauer data, and/or simulation of XANES spectra, are required to give a unique determination.

5. Conclusions

We have successfully validated the methodology of Wilke *et al.* (Petit et al. 2001; Wilke et al. 2001), for analysis of weak pre-edge features in Fe K-edge XANES for determination of Fe speciation, using data acquired from model compounds in a matter of hours on a commercially available laboratory X-ray spectrometer. Quantitative agreement was observed

between the total integrated intensity and centroid energy of the pre-edge features determined from laboratory and synchrotron data, and with previously published independent data. The primary sources of discrepancy in these parameters within our study were systematic error, arising from marginal difference in calibration of the absolute energy scale and underestimation of total integrated intensity due to lower signal to noise ratio in the laboratory data (which could be compensated, to an extent, by increased effective counting time). Therefore, for accurate speciation, data from a library of reference compounds should be established for the particular laboratory or synchrotron instrument. This proof of concept study has also clearly established the feasibility of data acquisition and analysis for relatively dilute Fe absorber concentrations. The rate of core-hole generation in our set up is not favourable for fluorescence data acquisition as a result of the low power 100W X-ray source, however, successful laboratory fluorescence XAS measurements using a 1.5 kW X-ray source were recently reported by Honkanen et al. 2019. Nevertheless, as we have demonstrated here, transmission mode XANES may be acquired from relatively dilute absorber concentrations without heroic data acquisition times, in favourable circumstances. Indeed, we have recently reported further exploitation this approach to speciation of Ce and U L₃ edge XANES, with absorber concentrations of only a few mol% (Mottram et al. 2020).

Acknowledgements. We are grateful for financial support from the Nuclear Decommissioning Authority and EPSRC under grant numbers EP/M026566/1, EP/S01019X/1, EP/N017870/1 and EP/R511754/1. This research utilised the HADES / MIDAS facility at The University of Sheffield established with financial support from EPSRC and BEIS, under grant EP/T011424/1. This research was undertaken, in part, at the DUBBLE beamline, BM 26, at the European Synchrotron Radiation Facility. We gratefully acknowledge G.T. Seidler and D.R. Mortensen for useful discussions in support of this study.

References

- ARNOLD H (1986) Crystal structure of FePO₄ at 294 and 20 K. *Zeitschrift für Kristallographie - Crystalline Materials* 177: 139–142
- BAJT S, SUTTON SR, DELANEY JS (1994) X-ray microprobe analysis of iron oxidation states in silicates and oxides using X-ray absorption near edge structure (XANES). *Geochimica et Cosmochimica Acta* 58: 5209-5214
- BAKER ML, MARA MW, YAN JJ, HODGSON KO, HEDMAN B, SOLOMON EI (2017) K- and L-edge X-ray Absorption Spectroscopy (XAS) and Resonant Inelastic X-ray Scattering (RIXS) Determination of Differential Orbital Covalency (DOC) of Transition Metal Sites. *Coordination Chemistry Reviews* 345: 182-208
- BAUM E, TREUTMANN W, BEHRUZI M, LOTTERMOSER W, AMTHAUER G (1988) Structural and magnetic properties of the clinopyroxenes NaFeSi₂O₆ and LiFeSi₂O₆. *Zeitschrift für Kristallographie* 183: 273–284
- BEARDEN JA, BURR AF (1967) Reevaluation of X-Ray Atomic Energy Levels. *Reviews of Modern Physics* 39: 125
- BERRY AJ, O'NEILL HS, JAYASURIYA KD, CAMPBELL SJ, FORAN GJ (2003) XANES calibrations for the oxidation state of iron in a silicate glass. *American Mineralogist* 88: 967-977
- BLACHUCKI W, CZAPLA-MASZTAFIAK, J, SA J, SZLACHETKO J (2019) A laboratory-based double X-ray spectrometer for simultaneous X-ray emission and X-ray absorption studies. *Journal of Analytical Atomic Spectrometry* 34: 1409-1415

- BORSBOOM M, BRAS W, CERJAK I, DETOLLENAERE D, GLASTRA VAN LOON D, GOEDTKINDT P, KONIJNENBURG M, LASSING P, LEVINE YK, MUNNEKE B, OVERSLUIZEN M, VAN TOL R, Vlieg E (1988) The Dutch-Belgian beamline at the ESRF. *Journal of Synchrotron Radiation* 5: 518-520
- DE GROOT F, VANKO G, GLATZEL P (2009) The 1s x-ray absorption pre-edge structures in transition metal oxides. *Journal of Physics Condensed Matter*: 21 104207
- DRÄGER G, FRAHM R, MATERLIK G, BRÜMMER O (1988) On the Multipole Character of the X-Ray Transitions in the Pre-Edge Structure of Fe K Absorption Spectra - An Experimental Study. *Physica Status Solidi B - Basic Research* 146: 287-294
- GALOISY L, CALAS G, ARRIO MA (2001) High-resolution XANES spectra of iron in minerals and glasses: structural information from the pre-edge region. *Chemical Geology* 174: 307-319
- GREENWOOD N, EARNSHAW A (1997) *Chemistry of the Elements*, 2nd Edition. Butterworth-Heinemann, Oxford pp 1-1342
- HAWTHORNE FC, UNGARETTI L, OBERTI R, CAUCIA F, CALLEGARI A (1993) The crystal chemistry of staurolite; 1. Crystal structure and site populations. *The Canadian Mineralogist* 31: 551-582
- HOLDEN WM, HOIDN OR, DITTER AS, SEIDLER GT, KAS J, STEIN JL, COSSAIRT BM., KOSIMOR SA, GUO JH, YE YF, MARCUS MA, FAKRA S (2017) A compact dispersive refocusing Rowland circle X-ray emission spectrometer for laboratory, synchrotron, and XFEL applications. *Reviews of Scientific Instruments* 88: 073904

- HONKANEN AP, OLLIKKALA S, AHOPELTO T, KALLIO AJ, BLOMBERG M, HUOTARI S (2019) Johann-type laboratory-scale x-ray absorption spectrometer with versatile detection modes. *Reviews of Scientific Instruments* 90: 033107
- JAHрман EP, HOLDEN WM, DITTER AS, MORTENSEN DR, SEIDLER GT, FISTER TT, KOZIMOR SA, PIPER LFJ, RANA J, HYATT NC, STENNETT M (2019) An improved laboratory-based x-ray absorption fine structure and x-ray emission spectrometer for analytical applications in materials chemistry research. *Reviews of Scientific Instruments* 90: 024106.
- JOSEPH K, STENNETT MC, HYATT NC, ASUVATHRAMAN R, DUBE CL, GANDY AS, KUTTY KVG, JOLLEY K, RAO PRV, SMITH R (2017) Iron phosphate glasses: Bulk properties and atomic scale structure. *Journal of Nuclear Materials* 494: 342-353.
- KRAUSE MO, OLIVER J H (1979) Natural widths of atomic K and L levels, $K\alpha$ X-ray lines and several KLL Auger lines. *Journal of Physical and Chemical Reference Data* 8: 320-338
- MALZER W, GROTZSCH G, GNEWKOW R, SCHLESIGER C, KOWALEWSKI F, VAN KUIKEN B, DEBEER S, KANNGIESSER B (2018) A laboratory spectrometer for high throughput X-ray emission spectroscopy in catalysis research. *Reviews of Scientific Instruments* 89: 113111
- MORTENSEN DR, SEIDLER GT, DITTER AS, GLATZEL P (2016) Benchtop Nonresonant X-ray Emission Spectroscopy: Coming Soon to Laboratories and XAS Beamlines Near You? *Journal of Physics Conference Series* 712: 012036
- MORTENSEN DR, SEIDLER GT (2017) Robust optic alignment in a tilt-free implementation of the Rowland circle spectrometer. *Journal of Electron Spectroscopy and Related Phenomena* 215: 8-15

- MOTTRAM LM, DIXON WILKINS MC, BLACKBURN LR, OULTON T, STENNETT MC, SUN SK, CORKHILL CL, HYATT NC (2020), A Feasibility Investigation of Laboratory Based X-ray Absorption Spectroscopy in Support of Nuclear Waste Management. *MRS Adv* 5: 27-35.
- NEMETH Z, SZLACHETKO J, BAJNOCZI EG, VANKO G (2016) Laboratory von Hamos X-ray spectroscopy for routine sample characterization. *Reviews of Scientific Instruments* 87: 103105
- PETIT PE, FARGES F, WILKE M, SOLÉ VA, Determination of the iron oxidation state in Earth materials using XANES pre-edge information, *Journal of Synchrotron Radiation*, 8, 2001, 952-954
- RAVEL B, NEWVILLE M, (2005) ATHENA, ARTEMIS, HEPHAESTUS: data analysis for X-ray absorption spectroscopy using IFEFFIT. *Journal of Synchrotron Radiation* 12: 537-541
- SCHLESIGER C, ANKLAMM L, STIEL H, MALZER W, KANNGIESSER B (2015) XAFS spectroscopy by an X-ray tube based spectrometer using a novel type of HOPG mosaic crystal and optimized image processing. *Journal of Analytical Atomic Spectrometry* 30: 1080-1085.
- SEIDLER GT, MORTENSEN DR, REMESNIK AJ, PACOLD JI, BALL NA, BARRY N, STYCZINSKI M, HOIDN OR (2014) A laboratory-based hard x-ray monochromator for high-resolution x-ray emission spectroscopy and x-ray absorption near edge structure measurements. *Reviews of Scientific Instruments* 85: 113906
- SEIDLER GT, DITTER AS, BALL NA, REMESNIK AJ (2016) A Modern Laboratory XAFS Cookbook. *Journal of Physics Conference Series* 712: 012015

- SMYTH JR (1975) High Temperature Crystal Chemistry of Fayalite. *American Mineralogist* 60: 1092-1097
- STERN EA, KIM K, (1981) Thickness effect on the extended-x-ray-absorption-fine-structure amplitude. *Physical Review B* 23: 3781-3787
- TAYLOR KG, KONHAUSER KO (2011) Iron in Earth Surface Systems: A Major Player in Chemical and Biological Processes. *Elements* 7: 83-87
- WAYCHUNAS GA, APTED MJ, BROWN GE (1983) X-ray K-edge Absorption-Spectra of Fe Minerals and Model Compounds - Near-Edge Structure. *Physics and Chemistry of Minerals* 10: 1-9
- WESTRE TE, KENNEPOH P, DEWITT JG, HEDMAN B, HODGSON KO, SOLOMON EI (1997) A Multiplet Analysis of Fe K-Edge 1s f 3d Pre-Edge Features of Iron Complexes. *Journal of the American Chemical Society* 119: 6297-6314
- WILKE M, FARGES F, PETIT PE BROWN, GE, MARTIN F (2001) Oxidation state and coordination of Fe in minerals: An Fe K-XANES spectroscopic study, *American Mineralogist* 86: 714-730
- WOOD BJ, VIRGO D (1989) Upper mantle oxidation state: Ferric iron contents of Iherzolite spinels by ^{57}Fe Mössbauer spectroscopy and resultant oxygen fugacities. *Geochimica et Cosmochimica Acta* 53: 1277-1291
- ZEESHAN F, HOSZOWSKA J, LOPERETTI-TORNAY L, DOUSSE JC (2019) In-house setup for laboratory-based x-ray absorption fine structure spectroscopy measurements. *Reviews of Scientific Instruments* 90: 073105