

This is a repository copy of *Whole-cell paper strip biosensors to semi-quantify tetracycline antibiotics in environmental matrices*.

White Rose Research Online URL for this paper:

<https://eprints.whiterose.ac.uk/165873/>

Version: Accepted Version

---

**Article:**

Ma, Zhao, Liu, Juan, Sallach, J. Brett orcid.org/0000-0003-4588-3364 et al. (2 more authors) (2020) Whole-cell paper strip biosensors to semi-quantify tetracycline antibiotics in environmental matrices. *Biosensors and Bioelectronics*. 112528. pp. 1-26. ISSN 0956-5663

<https://doi.org/10.1016/j.bios.2020.112528>

---

**Reuse**

This article is distributed under the terms of the Creative Commons Attribution-NonCommercial-NoDerivs (CC BY-NC-ND) licence. This licence only allows you to download this work and share it with others as long as you credit the authors, but you can't change the article in any way or use it commercially. More information and the full terms of the licence here: <https://creativecommons.org/licenses/>

**Takedown**

If you consider content in White Rose Research Online to be in breach of UK law, please notify us by emailing [eprints@whiterose.ac.uk](mailto:eprints@whiterose.ac.uk) including the URL of the record and the reason for the withdrawal request.

1 **Whole-Cell Paper Strip Biosensors to Semi-quantify**  
2 **Tetracycline Antibiotics in Environmental Matrices**

3 Zhao Ma <sup>a,1</sup>, Juan Liu <sup>a,1</sup>, J. Brett Sallach <sup>b</sup>, Xiaojie Hu <sup>a</sup>, Yanzheng Gao <sup>a,\*</sup>

4  
5 <sup>a</sup> Institute of Organic Contaminant Control and Soil Remediation, College of  
6 Resources and Environmental Sciences, Nanjing Agricultural University, Nanjing  
7 210095, P. R. China

8 <sup>b</sup> Department of Environment and Geography, University of York, Heslington, York,  
9 YO10 4DU, UK

10  
11 **\*Corresponding author:**

12 Yanzheng Gao, Address: Weigang Road 1, Nanjing 210095 China. Tel: +86-25-84395019.

13 ORCID No.: 0000-0002-3814-3555. E-mail: gaoyanzheng@njau.edu.cn.

14  
15  
16 <sup>1</sup>These authors contribute equally to this paper.

17  
18  
19 **Submit to Biosensors and Bioelectronics**

22 **ABSTRACT**

23 A novel, low-cost, and portable paper strip biosensor was developed for the detection of  
24 tetracycline antibiotics. *Escherichia coli*/pMTLacZ containing the tetracycline-mediated  
25 regulatory gene used as recognition elements with  $\beta$ -galactosidase as the reporter protein  
26 was designed and applied to cheap and portable Whatman filter paper as the carrier to  
27 prepare this paper strip biosensor. The detection process was optimized by using EDTA  
28 and polymyxin B as a sensitizer to improve the accuracy of detection for complicated  
29 matrices. The paper strip biosensor was suitable for tetracycline concentrations in the  
30 range of 75–10000  $\mu\text{g/L}$  in water and 75–7500  $\mu\text{g/L}$  in soil extracts. Detection limits of  
31 5.23–17.1  $\mu\text{g/L}$  for water and 5.21–35.3  $\mu\text{g/kg}$  for the EDTA soil extracts were achieved at  
32 a response time of 90 min. The standard deviation (SD) of detected values by the  
33 biosensor paper strip compared to those determined by HPLC was between 13.4–59.6%  
34 for tetracycline and 2.01–33.5% for oxytetracycline in water and was between  
35 6.22–72.8% for tetracycline and 5.90–43.4% for oxytetracycline in soil. This suggests that  
36 the paper strip biosensor was suitable for detecting both tetracycline and oxytetracycline  
37 in water, and could provide a suitable detection for extractable oxytetracycline in soils.  
38 Therefore, this biosensor provides a simple, economical, and portable piece of field kit for  
39 on-site monitoring of tetracyclines in a variety of environmental samples, such as pond  
40 water and agricultural soil that are susceptible to tetracycline pollution from feed additives  
41 and fertilization with livestock manure.

42

43 **Keywords:** Paper strip; Tetracyclines; Detection; Semi-quantity; Water; Soil

44

45

46

## 47 **1. Introduction**

48 Antibiotics are largely used in human medicine, animal husbandry, agriculture, and  
49 aquaculture (Hoa et al. 2011; Teuber 2001). The rampant usage of antibiotics has led to  
50 their ubiquitous occurrence in environmental compartments, including water, soil, and  
51 sediment impacted by wastewater, sewage sludge, or livestock manure, etc (Berendonk et  
52 al. 2015; Gothwal and Shashidhar 2015; Liu et al. 2017). Until now, over 30 types of  
53 antibiotics, including those from the tetracycline, sulfonamide, macrolide, and quinolone  
54 classes of antibiotics, have been detected with concentrations typically at microgram per  
55 liter levels in pond waters (Limbu et al. 2018; Liu et al. 2017; Rico et al. 2017) and  
56 microgram per kilogram levels in soils and sediment (Hu et al. 2010; Kumar et al. 2005;  
57 Liu et al. 2009). However, in heavily impacted agricultural waters, concentrations have  
58 been measured at the milligram per liter level (Bartelt-Hunt et al. 2011; Peak et al. 2007;  
59 Zilles et al. 2005). One major concern is that environmental exposure to these antibiotics  
60 can induce resistance in native bacteria, contributing to the development of the  
61 environmental resistome, and resulting in lower effectiveness of antibiotics in the  
62 treatment of bacterial infections.

63 Preventing the environmental introduction of antibiotics is an ideal way to reduce the  
64 proliferation of antibiotic resistant bacteria and antibiotic resistance genes (Berendonk et  
65 al. 2015; Gao et al. 2018; Rodriguez-Mozaz et al. 2015; Zhu et al. 2013). Among the  
66 antibiotics, tetracyclines are essential in modern intensive agriculture production and  
67 widely used in livestock and mariculture farming (Gu et al. 2020; Scarano et al. 2018).  
68 Currently, there is a growing effort to reduce their input and impact (Du and Liu 2012; Hu  
69 et al. 2010; Kumar et al. 2005; Liu et al. 2017; Thiele-Bruhn 2003). Quick, easy, and  
70 cost-effective methods are urgently needed to monitor and support the management  
71 practices for drug control during food production as well as following their introduction

72 into water and soil.

73 Currently, numerous antibiotic detection methods have been developed, most of  
74 which being chemical analytical methods utilizing high-performance liquid  
75 chromatography and mass spectrometry for the extraction and separation of antibiotics  
76 from complex environmental samples. These traditional methods require complicated,  
77 time-consuming, reagent heavy processing and expensive instrumentation that relies upon  
78 the user's expertise to interpret results (Batt and Aga 2005; Hamscher et al. 2002).  
79 Recently, paper test strips have been developed for the detection of bioactive contaminants  
80 like antibiotics. Most of these paper sensors are based on aptamers or monoclonal  
81 antibodies as recognition elements with nanofibers or gold nanoparticles acting as  
82 transducers (Abbas et al. 2013; Ferreira et al. 2015; Liana et al. 2012; Ornatska et al.  
83 2011). Nevertheless, some deficiencies of these sensors have been recognized and include  
84 time-consuming, expensive, cumbersome fabrication (Gullapalli et al. 2010) or  
85 insufficient sensitivity due to shifting ion level, pH, temperature, or light interference  
86 (Ahmed et al. 2014; Chaiyo et al. 2015; Hossain et al. 2009; Quesada-González and  
87 Merkoçi 2015). All these factors have impeded the practical application of existing sensors  
88 for antibiotic detection in soils and water.

89 Whole-cell biosensors provide a self-contained portable sensing system based on  
90 genetically engineered whole cells that physically are adsorbed on filter-paper strips for  
91 on-site semiquantitative visual monitoring of N-acylhomoserine lactones (AHLs) agonists  
92 in a test sample (Struss et al. 2010). This paper strip biosensor could serve as a simple and  
93 economical portable piece of field kit for on-site monitoring of AHLs in various types of  
94 environmental samples. So far, the efficacy of these antibiotic biosensors have only been  
95 demonstrated in preliminary research for the detection of antibiotics in water and soils  
96 under laboratory conditions (Ma et al. 2020). Studies on antibiotic colorimetric strips

97 using whole-cell biosensors for on-site semiquantitative visual testing are not available.

98 In this study, we reported the development of a self-contained sensing system  
99 deployed on a paper strip for the detection of tetracyclines in environmental samples. This  
100 sensing system was based on genetically engineered bacterial cells that were directly dried  
101 on filter paper strips. These bacterial sensing cells employ  $\beta$ -galactosidase as the reporter  
102 protein, which can serve visual detections for antibiotics by using a chromogenic enzyme  
103 substrate (X-gal). The sensing system was validated by application in the detection of  
104 tetracyclines in water and soil. Paper strip biosensors allowed for visual, fast, convenient,  
105 and dose-dependent monitoring of tetracyclines in tested samples, thus demonstrating their  
106 value as a portable tool for on-site analysis of environmental samples.

107

## 108 **2. Methods**

### 109 *2.1 Chemicals*

110 All chemicals used in this study are described in Supplemental [Text S1](#) and [Table S1](#)  
111 of Supporting Information ([SI](#)).

### 112 *2.2 Plasmids construction*

113 The gene sequences corresponding to the pMT fragment from the  
114 tetracycline-mediated regulatory system of *Staphylococcus rostri* strain RST11:Tn916 and  
115 transposon Tn10 were isolated from plasmid pMTmCherry using polymerase chain  
116 reaction (PCR) with primers ([Table S2](#), [Table S3](#)). The *lacZ* fragment encoding  
117  $\beta$ -galactosidase was PCR-amplified by the primers ([Table S3](#)) from the pUC19 plasmid  
118 ([Table S2](#)). The pMTLacZ plasmid was prepared by recombining the *lacZ* fragment and  
119 pMT fragment using Trelief™ SoSoo cloning kit. The recombined plasmids were  
120 subsequently transformed into competent *Escherichia coli* BL21 cells ([Table S2](#))  
121 according to molecular cloning protocols and then verified using highly specific primers

122 (Table S4) (Sambrook et al. 1989). The transformed cells were sifted via culturing on  
123 Lysogeny broth (LB) agar plates containing 100 mg/L ampicillin and 20 mg/L X-gal at  
124 37 °C overnight for screening *E. coli* BL21/pMTLacZ.

### 125 2.3 Fabrication of paper strips

126 Paper strips were prepared as described by Struss *et al.* with some modifications  
127 (Struss et al. 2010). Biosensor cells were cultured for about 4–5 hours at 37 °C and at 150  
128 r/min in the LB medium (containing 100 mg/L ampicillin), resulting in an OD<sub>600</sub> of  
129 0.450–0.500. Cells were centrifuged at 4,000 × *g* for 10 min and resuspended in 1/4  
130 lysogeny broth with 10% lactose and polymyxin B. The biosensor cell suspension (50 µL)  
131 was spotted on Whatman filter paper strips (1 × 4 cm), dried for 10 min at room  
132 temperature and then subsequently dried by vacuum freeze-drying. These paper strips  
133 were stored at -20 °C for further study.

### 134 2.4 Tetracycline analysis in water

135 Standard solutions of six tetracyclines were prepared individually at fourteen  
136 concentration levels (0, 10, 25, 50, 75, 100, 250, 500, 750, 1000, 2500, 5000, 7500 and  
137 10000 µg/L) in sterilized Milli-Q water. Each tetracycline solution (100 µL) or  
138 environmental water sample was mixed with 900 µL LB medium (containing 100 µg/mL  
139 ampicillin) in a polyethylene tube. Previously prepared paper strips were inserted in these  
140 culture tubes and incubated at 37 °C without shaking for 90 min. Paper strips were then  
141 taken out of the culture tubes and prevented from drying. After, 10 µL of X-gal substrate  
142 solution (50 g/L) in DMF was added on the biosensor cell spot. The paper strip was  
143 shielded from light at 37 °C for 90 min for color development. A Sony α7 III digital  
144 camera (Sony, Tokyo, Japan) with Sony shots (20 mm F1.8, Tokyo, Japan) was used for  
145 taking RAW images of the strips (Struss et al. 2010).

146 The color intensities, rather than the size of the blue area, an artifact of differences in

147 the dispersive size of the X-gal color developing agent, were measured using the software  
148 ImageJ (National Institutes of Health, Bethesda, Maryland, US)  
149 (<https://imagej.net/Downloads>) upon acquired digital images above and used to determine  
150 tetracycline concentrations. The measurement settings of the images were set to mean gray  
151 value in ImageJ that converts 100% white as 255 and 100% black as zero. A rectangle  
152 section (1 × 1 mm area) in each image was drawn around a spot on the strip and measured  
153 using the selection tool in ImageJ software. A background measurement was implemented  
154 of the same size on the bare paper strip, to normalize for slightly different color intensities  
155 due to changing illumination while these pictures were obtained in the field. The paper  
156 strip biosensor-based calibration was confirmed with the tetracycline concentration  
157 quantified by high-performance liquid chromatography (HPLC) (Fig. S1). The limit of  
158 detection (LOD) of a biosensor is usually calculated as the concentration at which  
159 biosensor signal to noise ratio is above 3. Therefore, while measuring the pixel density  
160 changes in samples devoid of tetracyclines (buffer only), biosensor noise was determined  
161 and used for the calculation of the LOD for the paper strip biosensor (S/N=3). The  
162 linearity ranges of the biosensors paper strip were calculated according to the r values of  
163 the standard curves greater than 0.800 (Burrows and Watson 2015). The obtained standard  
164 curves were then used for analyses of tetracyclines in water samples (W<sub>1-20</sub>).

165 Twenty water samples were obtained from Nanjing fishponds (Physicochemical  
166 properties of the water samples are provided in Table S5 of SI). The sampling sites of  
167 water samples were labeled on the map of Nanjing and these samples were mainly  
168 collected around Xuanwu lake and Yueya lake of Nanjing (Fig. S4). A random dose of  
169 either tetracycline (W<sub>1-10</sub>) and oxytetracycline (W<sub>10-20</sub>) was added to the twenty water  
170 samples (W<sub>1</sub>–W<sub>20</sub>), which was used to simulate polluted pond water from the input of feed  
171 additives used in aquaculture. These samples were aged for 30 days under outdoor



172 conditions prior to analysis. HPLC (LC-20AT, Shimadzu Co., Kyoto, Japan, Detailed  
173 process in SI of Fig. S2) was first used to screen and quantify tetracycline concentrations.  
174 The estimated concentration of tetracyclines was detected by paper strip and calculated  
175 using the fourteen-point paper strip calibration described above.

#### 176 *2.5 Tetracyclines analysis in soil*

177 A volume of 100  $\mu$ L of each of the soil matrix calibrants (see Supplemental Text S2  
178 for the preparation process) was added to 900  $\mu$ L of LB medium in culture tubes in  
179 triplicate. The detection procedure was performed as described for water. A dose-response  
180 curve using standard tetracyclines solutions prepared in soil extracts was obtained by  
181 paper strip biosensors in each analytical run as well as HPLC as a reference for  
182 comparison.

183 Twenty tetracycline-contaminated Inceptisol samples were obtained from a test field  
184 at Nanjing Agricultural University (Nanjing, China). The physicochemical properties of  
185 Inceptisol are given in Table S6. Ten soil samples (S<sub>1-10</sub>) were obtained from the  
186 tetracycline test field which received tetracycline exposures for at least one year, and ten  
187 soil samples (S<sub>11-20</sub>) were obtained from another test field that was contaminated with  
188 oxytetracycline for at least one year. Each processed soil extract (100  $\mu$ L) (i.e., the EDTA  
189 soil extract, see Supplemental Text S3 for the pretreatment process of soils) was analyzed  
190 by the methods described previously using the paper strip biosensor. The concentration  
191 was then determined by colorimetrics based on the matrix matched calibration curve  
192 described above.

193


### 194 **3. Results and discussion**

#### 195 *3.1 Biosensor construction and paper strip production*

196 The schematic of pMTLacZ plasmids used in this study is shown in Fig. 1A. The *lacZ*

197 gene and T7 gene were fused to obtain *lacZ*-T7 gene (Fig. 1B). To construct this biosensor  
198 for the sensing of tetracyclines, the pMT gene (Fig. 1B), *lacZ*-T7 gene (Fig. 1B) and T7  
199 gene (Fig. 1B) were used to construct the biosensor plasmids by DNA homologous  
200 recombination. Additionally, the recombinant plasmid was further verified by PCR with  
201 specific primers, and the amplicon lengths were consistent with those expected (pMTLacZ  
202 3590 bp) (Fig. 1C). As shown in Fig. 1a, *E. coli* BL21 strain containing a pMTLacZ  
203 plasmid produced the blue colony with X-gal when exposed to tetracycline. The  
204 expression of the reporter gene is under tight transcriptional control of the tetracycline  
205 repressor (*tetR*) on the plasmid (pMTLacZ, Fig. 1A and Fig. 1D). Binding of tetracycline  
206 to *tetR* abolishes the binding of this gene to two operator sites (*tetO*) and thus allows  
207 expression of the *lacZ* gene (Fig. 1D) and translation of  $\beta$ -galactosidase (Orth et al. 2000).  
208 X-gal can be degraded by  $\beta$ -galactosidase, which then produces the blue signal  
209 (5,5'-dibromo-4,4'-dichloro-indigo, Fig. 1E). The induction results of tetracyclines  
210 revealed that exposure to an increased concentration of antibiotic can increase the enzyme  
211 activity response of the biosensor with a dose-related effect (Fig. S3, Detailed illustration  
212 in SI).

213 Based on this character of the constructed bacterium, the paper strip biosensor was  
214 designed as follows (Fig. 1F). The biosensor cells were cultured in the LB medium,  
215 centrifuged and resuspended in 1/4 LB with 10% lactose and PMB (Fig. 1F, step i-iii). The  
216 suspension was spotted on Whatman filter paper strips (1 × 4 cm, Fig. 1F, step iv), then  
217 dried by vacuum freeze-drying. The paper strip biosensor was immersed in LB broth with  
218 samples at 37 °C for 1.5 h (Fig. 1F, step v). Once removed, the color development reagent  
219 (X-gal) was added to the biosensor cells (Fig. 1F, step vi) before imaging and post-image  
220 processing (Fig. 1F, step vii).



221  
 222 **Fig. 1** The construction of the recombinant plasmids. Schematic of the recombinant plasmid  
 223 (pMTLacZ) and the fluorescence response of the bacteria (*E. coli* BL21/pMTLacZ) induced by 20  
 224 mg/L tetracycline (TC) (A), Agarose gel electrophoresis of fused gene fragment amplified by PCR  
 225 (M<sub>1</sub>-DNA marker DL5000, 1-*lacZ*, 2-T7, 3-*lacZ*-T7, 4-pMT, M<sub>2</sub>-*Trans2K*<sup>®</sup> Plus II DNA Marker) (B),  
 226 Agarose gel electrophoresis of cloning gene verified by PCR (M-DNA marker DL5000, 1-pMTLacZ  
 227 partial fragment) (C). Genetic organization and mechanism of tetracycline-regulated TC-resistance  
 228 determinant (D). The coupled enzyme reactions were catalyzed by β-galactosidase producing the blue  
 229 signal (E). Tetracycline semi-quantification processing by whole-cell paper strip biosensor (F).  
 230 Biosensor cultivation (i), preparation of paper strip biosensor (ii-iv), Semi-quantitative analysis of  
 231 samples using biosensor (v-vii).  
 232


233

234

235

236

237

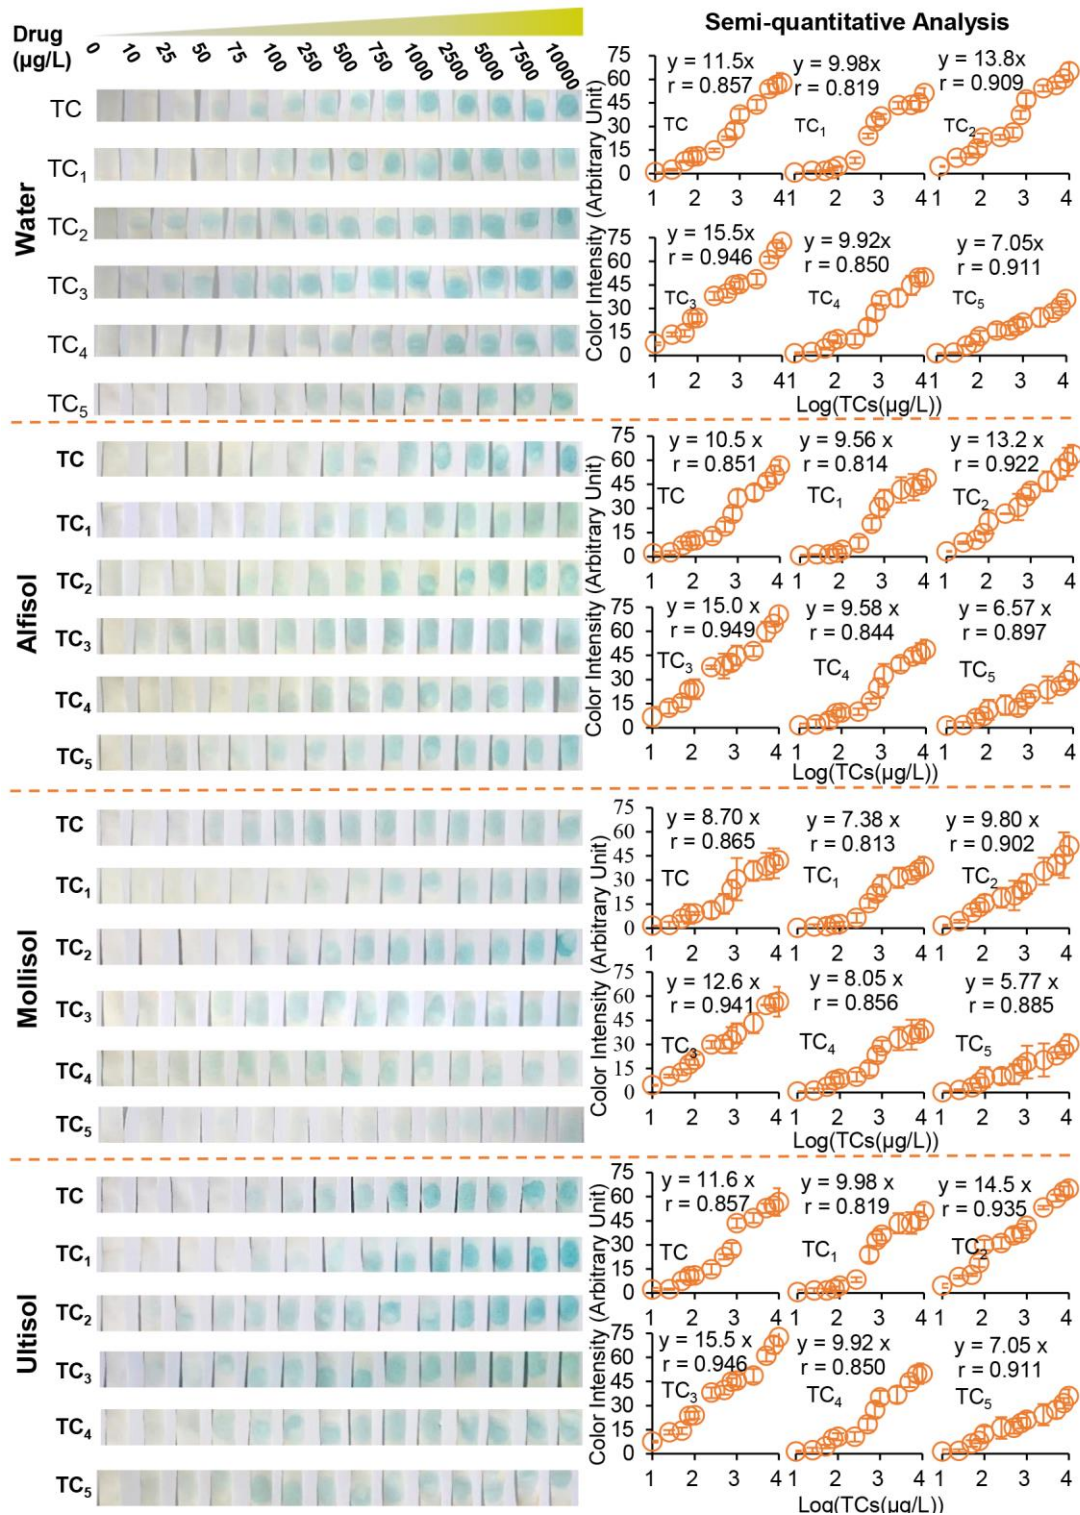

239  
 240 **Fig. 2** Matrix matched calibration of paper strip biosensors for water and soil extracts and the  
 241 correlations between spiked tetracycline concentrations in and color intensity measured using the  
 242 software ImageJ upon digital image acquisition. TC, TC<sub>1</sub>, TC<sub>2</sub>, TC<sub>3</sub>, TC<sub>4</sub> and TC<sub>5</sub> denote tetracycline,  
 243 oxytetracycline, chlorotetracycline, deoxytetracycline, minocycline, and methacycline, respectively.

244 For semi-quantification of tetracycline concentrations in the samples, a 14-point

245 calibration was prepared for each of the six tetracycline compounds (tetracycline,  
246 oxytetracycline, chlorotetracycline, deoxytetracycline, minocycline, and methacycline)  
247 spiked in aquafarm water at concentrations ranging from 0–10,000 µg/L. An increase in  
248 blue color intensity was observed with increasing concentrations of tetracyclines (Fig. 2).  
249 The visual results of the paper strip biosensor were able to indicate low tetracycline  
250 concentrations down to 10 µg/L upon color development for 90 min. A good linear  
251 relationship between the color intensity and log value of tetracycline concentration in  
252 water was observed (Fig. 2,  $r > 0.850$ ,  $P < 0.01$ ). The concentration of each tetracycline in  
253 water as a function of the color intensity on the paper strip can be expressed as equation 1  
254 and 2 (Table S5, Detailed illustration in SI).

$$255 \quad \log TC = \alpha I \quad (1)$$

256 or

$$257 \quad TC = 10^{\alpha I} \quad (2)$$

258 where TC is the concentration of tetracycline, I is the color intensity detected by the  
259 paper strip biosensors and, and  $\alpha$  is the slope of standard curve (Values given in Fig. 2).  
260 Using the color intensity reading of the biosensors paper strip and Eq. (2), TC can be then  
261 calculated by I and  $\alpha$  (Fig. 2) obtained from their corresponding standard calibration curve.  
262 After 90 min incubation, good linearity in the range of 75–10000 µg/L were found by  
263 paper strip biosensors for six tetracyclines (Table 1). The detection limits of the biosensor  
264 method in water were between 5.23 and 17.1 µg/L for all types of soils and tetracyclines  
265 as determined by S/N ratio. The paper strip biosensor produced a slightly lower detection  
266 limit for chlorotetracycline (5.44 µg/L) and deoxytetracycline (5.23 µg/L) than for other

267 tetracyclines in water. In comparison, Zhu et al. (2010) obtained a detection limit of  
 268 0.20–0.28 µg/L for tetracyclines in groundwater by HPLC. Although the primary aim of  
 269 this study was to develop a paper strip biosensor for the onsite, high-throughput screening  
 270 of tetracyclines in water, it is conceivable that the detection limits achieved by HPLC  
 271 could also be achieved by the biosensor if concentration of the water samples was  
 272 conducted (Zhu et al. 2001).

273 **Table 1** Detection parameters of six tetracyclines measured by biosensors paper strip in water and soil  
 274 extracts (Alfisol, Mollisol, and Ultisol)

TCs	Water		Alfisol		Mollisol		Ultisol	
	DL (µg/L)	LR (µg/L)	DL (µg/L)	LR (µg/L)	DL (µg/L)	LR (µg/L)	DL (µg/L)	LR (µg/L)
TC	5.86	25-10000	5.88	25-5000	20.4	50-7500	5.32	50-10000
TC <sub>1</sub>	5.85	75-10000	5.95	75-10000	30.1	75-10000	5.76	75-7500
TC <sub>2</sub>	5.44	25-10000	5.78	25-7500	19.1	10-10000	5.68	25-10000
TC <sub>3</sub>	5.23	10-10000	5.67	25-10000	17.0	10-10000	5.21	25-10000
TC <sub>4</sub>	17.1	75-10000	23.4	25-10000	30.2	25-7500	15.4	50-7500
TC <sub>5</sub>	9.05	75-10000	35.3	10-10000	28.4	25-7500	12.6	10-7500

275 TCs, TC, TC<sub>1</sub>, TC<sub>2</sub>, TC<sub>3</sub>, TC<sub>4</sub> and TC<sub>5</sub> are tetracyclines, tetracycline, oxytetracycline, chlorotetracycline,  
 276 deoxytetracycline, minocycline, and methacycline, respectively. DL and LR are detection limit and Linear range,  
 277 respectively.


278 The results above demonstrated the capacity of paper strip biosensors for  
 279 semi-quantitative detection of tetracyclines in water samples. Extractable fractions of  
 280 tetracyclines in soils are often used to assess their bioavailability to biota and their  
 281 mobility through soil profiles (Ikehata et al. 2006; Li et al. 2016; Liu et al. 2014). The  
 282 EDTA extractable fraction of tetracyclines can be used to evaluate their corresponding  
 283 environmental and health risks in soils (Bergan et al. 1973; Cipullo et al. 2018; Hansen  
 284 and Sørensen 2001). Therefore, further validation of the dose-response curves of six  
 285 tetracyclines from soil extracts using the paper strip biosensor was carried out using a  
 286 matrix matched approach of spiked soil extracts from three different soils. The sensitivity  
 287 of tetracyclines in soil extracts, as measured by the color intensity of the paper strip

288 biosensor response decreased from Ultisol and Alfisol to Mollisol (Fig. 2). The visual  
289 detection limit of the paper strip in soil extracts was between 25 and 100  $\mu\text{g/L}$  for all of  
290 the soils and tetracycline compounds. Measurement of the color intensities using  
291 appropriate software were shown to enhance sensitivity (Fig. 2). Image analysis indicated  
292 that the logarithmic concentration of each tetracycline in the soil extracts as a function of  
293 the color intensity followed also followed equation 1 ( $r > 0.813$ ,  $P < 0.01$ ) (Fig. 2). A good  
294 linearity in the range of 75–7500  $\mu\text{g/L}$  was determined for the paper strip biosensors for  
295 all six of the tetracyclines in the soil extracts (Table 1). The detection limits of  
296 tetracyclines in the EDTA-extracts of Inceptisol, Mollisol, and Ultisol were 5.67–35.3,  
297 17.0–30.2, and 5.21–15.4  $\mu\text{g/L}$  for this biosensor method (Table 1). Similar to the water,  
298 chlorotetracycline and deoxytetracycline showed the lowest paper strip biosensor  
299 detection limit in all three soil extracts whereas minocycline and methacycline were  
300 highest at 5.21  $\mu\text{g/L}$  in all three soil extracts. Overall, a lower limit of detection was  
301 observed in EDTA-extracts from Ultisol than either Inceptisol or Mollisol. The detection  
302 limits of the EDTA-extractable tetracyclines in three soils was calculated as  $DL = (DL_{SE}$   
303  $\times 1 \text{ mL})/1 \text{ g}$  ( $DL_{SE}$  denote the detection limit of tetracyclines in soil EDTA-extracts). So,  
304 the detection limit of the biosensor method for EDTA-extractable tetracyclines in three  
305 soil follow the same principles (5.21–30.2  $\mu\text{g/kg}$ , TableS7).

306

307

308

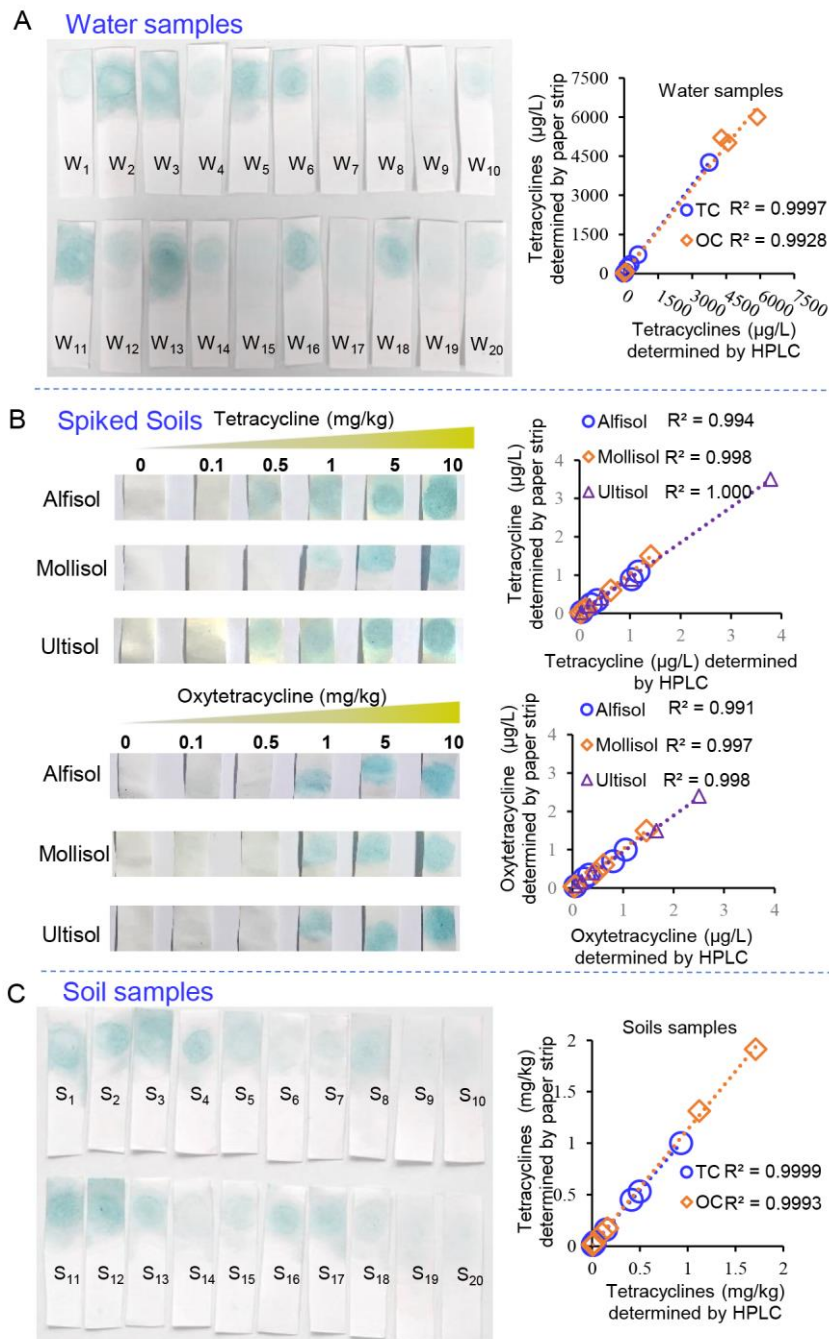

310

311 **Fig. 3** Tetracycline (TC) and oxytetracycline (OC) semi-quantitation in twenty water samples (A) and  
 312 twenty soil samples (B) and tetracyclines-spiked soils (C) by whole-cell paper strip biosensors. Results  
 313 represent the average of triplicate assays whereby prepared whole cell paper strip biosensors were  
 314 incubated in soil extracts at 37 °C and color intensity measured using the software ImageJ upon digital  
 315 image acquisition.

316 The utility of the paper strip biosensor was verified with the analysis of real water



317 samples. For the samples collected from fishponds, the data (Fig. 3A) were almost  
318 identical to those obtained from water samples in laboratory, which indicates the sample  
319 matrices had a negligible effect on the sensitivity of the biosensors for tetracyclines. For  
320 twenty water samples collected from local fishponds in Nanjing (China), the paper strip  
321 biosensor indicated that tetracycline concentrations of W<sub>1</sub>–W<sub>10</sub> were 45.8, 3756, 609, 6.32,  
322 263, 144, 7.75, 15.4, 7.9 and 6.78 µg/L, respectively (Fig. 3A and Table S7). The  
323 tetracycline concentrations of W<sub>1</sub>–W<sub>10</sub> water samples measured by HPLC were 59.7, 4260,  
324 718, 9.26, 350, 230, 12.2, 24.3, 11.2 and 10.4 µg/L, respectively, and were slightly higher  
325 than the results generated by biosensor method. Standard deviations (between estimated  
326 tetracycline concentration by biosensors paper strip and that detected by HPLC, SD) in the  
327 analysis of the 10 samples were between 13.4–59.6%. Oxytetracycline concentrations of  
328 W<sub>11</sub>–W<sub>20</sub> water samples were 4288, 22.4, 5882, 10.7, 66.8, 4585, 13.7, 26.8, 10.8 and 15.2  
329 µg/L, respectively (see Fig. 3A and Table S7). The oxytetracycline concentrations of  
330 W<sub>11</sub>–W<sub>20</sub> water samples measured by HPLC were 5201, 30.2, 6000, 14.2, 78.3, 5001, 15.2,  
331 30.3, 11.3 and 17.0 µg/L, respectively, and again were higher than the detected values by  
332 paper strip. The SD in the analysis of 10 samples contained oxytetracycline were  
333 2.01–33.5% (Fig. 3A and Table 2).

334

335

336

337 **Table 2** Tetracycline (TC) and oxytetracycline (OC) semi-quantitative values in twenty water samples and  
338 twenty soil samples by whole-cell paper strip biosensors

Sample	Cl	PC (mg/kg)	HC (mg/kg)	SD (%)
W <sub>1</sub>	19.1	45.8	59.7	30.2
W <sub>2</sub>	41.1	3756	4260	13.4
W <sub>3</sub>	32.0	609	718	17.8
W <sub>4</sub>	9.21	6.32	9.26	46.5
W <sub>5</sub>	27.8	263	350	32.9
W <sub>6</sub>	24.8	144	230	59.6
W <sub>7</sub>	10.2	7.75	12.2	57.8
W <sub>8</sub>	13.7	15.4	24.3	57.7
W <sub>9</sub>	10.3	7.90	11.2	42.4
W <sub>10</sub>	9.56	6.78	10.4	52.6
W <sub>11</sub>	36.3	4288	5201	21.3
W <sub>12</sub>	13.5	22.4	30.2	34.9
W <sub>13</sub>	37.6	5882	6000	2.01
W <sub>14</sub>	10.3	10.7	14.2	33.5
W <sub>15</sub>	18.2	66.8	78.3	17.2
W <sub>16</sub>	36.5	4585	5001	9.09
W <sub>17</sub>	11.3	13.7	15.2	11.4
W <sub>18</sub>	14.3	26.8	30.3	13.3
W <sub>19</sub>	10.3	10.6	11.3	5.71
W <sub>20</sub>	11.8	15.2	17.0	12.0
S <sub>1</sub>	28.3	0.498	0.532	6.86
S <sub>2</sub>	27.5	0.414	0.450	8.72
S <sub>3</sub>	31.2	0.928	0.100	7.78
S <sub>4</sub>	22.7	0.143	0.161	12.4
S <sub>5</sub>	15.3	0.029	0.041	42.5
S <sub>6</sub>	13.7	0.020	0.030	48.3
S <sub>7</sub>	10.3	0.009	0.016	72.8
S <sub>8</sub>	14.2	0.022	0.024	6.22
S <sub>9</sub>	9.5	0.008	0.011	41.3
S <sub>10</sub>	8.6	0.006	0.011	58.1
S <sub>11</sub>	30.9	1.71	1.91	11.7
S <sub>12</sub>	29.2	1.12	1.31	17.2
S <sub>13</sub>	13.2	0.024	0.030	25.4
S <sub>14</sub>	9.21	0.009	0.010	11.4
S <sub>15</sub>	9.79	0.011	0.013	25.3
S <sub>16</sub>	19.3	0.011	0.013	19.0
S <sub>17</sub>	21.1	0.163	0.172	5.90
S <sub>18</sub>	13.0	0.023	0.030	33.7
S <sub>19</sub>	7.26	0.006	0.008	43.4
S <sub>20</sub>	8.32	0.007	0.011	40.9

339 Color Intensity (CI, Arbitrary Unit), tetracycline concentration measured by paper strip biosensors (PC),  
340 concentration determined by HPLC (HC), and standard deviation (SD) between estimated tetracycline  
341 concentration, PC, and HPLC determined tetracycline concentration (HC) are presented.

342 When the values calculated by the biosensor were plotted against the HPLC derived  
343 concentrations, a strong linear relationship was established. ( $R^2 > 0.990$ , Fig. 3A). This  
344 shows that variation between results obtained from the two methods are not concentration  
345 dependent and suggests the potential to correct for the underestimated concentrations  
346 observed via biosensor analysis.

#### 347 *3.4 Analysis of extractable tetracyclines fraction in contaminated soil*

348 The paper strip biosensor was also validated for the analysis of the extractable  
349 tetracycline fraction in contaminated soils following the same extraction procedure from  
350 soil as described above. The results of the analysis in tetracycline and  
351 oxytetracycline-spiked soils revealed that the concentrations of extractable tetracycline  
352 measured by paper strip biosensors were closer to the values of extractable tetracycline  
353 concentration measured by HPLC (Fig. 3B). Two tetracyclines concentrations by  
354 whole-cell paper strip biosensors showed a good linear relationship with the  
355 concentrations of that of detection by HPLC ( $R^2 > 0.991$ ). The paper strip was further  
356 tested to detect tetracycline concentrations in soils sampled from a test field that were  
357 contaminated with either tetracycline or oxytetracycline. Using the paper strips, the  
358 extractable tetracycline concentration in S<sub>1</sub>-S<sub>10</sub> soils ranged from 0.006–0.498 mg/kg, (Fig.  
359 3C and Table 2), which were slightly lower than the concentrations measured by the  
360 HPLC method (0.011–0.532 mg/kg). The extractable oxytetracycline concentrations in  
361 S<sub>11</sub>-S<sub>20</sub> soils measured by paper strip biosensors ranged from were 0.006–1.71 mg/kg  
362 which were very similar to the concentrations measured by HPLC (0.008–1.91 mg/kg).  
363 The SD values of the extractable tetracycline in soils measured by the paper strip

364 biosensor S<sub>1</sub>-S<sub>10</sub> (6.86–72.8%) were greater than the SD values of the extractable  
365 oxytetracycline in S<sub>11</sub>-S<sub>20</sub> soils (5.90–43.4%). However, both SDs provide adequate  
366 reproducibility for a semi-quantitative method. The same as for water, a strong linear  
367 relationship existed between the concentrations of both compounds determined by paper  
368 strip biosensors and HPLC ( $R^2 > 0.999$ , Fig. 3C and Table 2). Combined with no  
369 observable matrix interferences, these results confirm that these paper strip biosensors  
370 provide reliable semi-quantitative evaluation of tetracycline concentrations from soil  
371 extracts.

### 372 3.5 Advantages

373 The paper strip biosensors include greater ability to accommodate the variation of  
374 environmental conditions in water or soil, such as a wide range of ionic strengths, pH  
375 (4–8), and temperature (Iglesias et al. 2009) that is hard to overcome the impact other  
376 types of paper strip sensors such as those based on immunochromatographic lateral flow  
377 and immobilization of antibodies. This biosensor is more robust and has an excellent  
378 capacity to endure various environmental conditions, such as those expected in pond water  
379 and agricultural soil where contamination with tetracycline antibiotics is commonly  
380 associated with the utilization of feed additives in aquaculture and the use of livestock  
381 manure as a soil fertilizer amendment.

382 In this study, the construction of *Escherichia coli*/pMTLacZ for whole-cell biosensor  
383 was similar to that of *Escherichia coli*/pMTGFP and *Escherichia coli*/pMTmcherry from  
384 our previous study (Ma et al. 2020). These cellular reporters can rapidly and accurately  
385 detect tetracyclines in water or soil. However, cost effective and readily available  
386 Whatman filter paper was utilized as the carrier for the biosensor scaffolding (Fig. 1),  
387 which has substantially greater portability and is more economical than the 96-microwell  
388 plate method described in previous studies (Wang et al. 2010; Zou et al. 2018). Biosensor

389 paper strips were produced by a simple culture process (3 hours at 37 °C with vigorous  
390 shaking at 150 r/min) in cheap media (Lysogeny Broth), which dramatically reduces  
391 analysis cost. This semi-quantitative method has adequate sensitivity and high selectivity,  
392 only detecting tetracycline antibiotics, and requires minimal sample pretreatment. This  
393 paper strip biosensor offers a lower analysis cost and little instrumental expertise  
394 compared to conventional analytical methods (gas chromatography, liquid  
395 chromatography, mass spectrometry) (Aga et al. 2016; Arefev et al. 1987). Meanwhile,  
396 developing EDTA solvent extraction for the detection of tetracyclines in soils is an  
397 inexpensive, easily accessible and environmentally-friendly method compared to many  
398 common methods which use organic solvents needed to perform chromatographic  
399 separations (Batt and Aga 2005; Hamscher et al. 2005). The combination of EDTA and  
400 polymyxin B as the agent to sensitize this material resulted in significantly improve  
401 method precision and accuracy (Belkin 2003; Parlanti et al. 2000).

402 At present, portable colorimeters and office scanners pixelated by GIMP software into  
403 an RGB profile can evaluate the color intensity of the paper strip, but it's exorbitant for  
404 onsite application and not nearly as portable as reagent kits. In our study, optical changes  
405 of the sensor were acquired by a digital camera and analyzed by Image J software that  
406 enhanced the portability of these paper strip kits while vastly reducing the expense of  
407 antibiotic detection. Based on the image processing described in this study, the color  
408 analysis software could be developed as a mobile phone APP to directly capture and  
409 analyze images and output detection results which would increase user-friendliness while  
410 further decreasing analysis time.

#### 411 **4. Conclusion**

412 We have developed a self-contained portable sensing system based on genetically  
413 engineered whole-cells physically adsorbed on filter-paper strips for on-site

414 semiquantitative visual monitoring of tetracyclines in environmental samples. Additionally,  
415 we demonstrate their ability to provide quantitative measurements by means of digital  
416 image analysis. This novel filter-paper strip biosensor method obtained a quantification  
417 range of 75–10000  $\mu\text{g/L}$  with detection limits of 5.23–17.1  $\mu\text{g/L}$  for 6 tetracycline  
418 antibiotics in water and a detection limit of 5.21–35.3  $\mu\text{g/kg}$  for the EDTA-extractable  
419 tetracyclines from three soils. This study describes a fast and convenient method for the  
420 detection of tetracyclines, which could be employed for first-level screening of a variety of  
421 environmentally and clinically relevant samples. A filter-paper-based biosensor provides  
422 easy transportation and storage, and does not require instrumentation or trained personnel;  
423 therefore, it could be a component of a simple and inexpensive field kit.

424

#### 425 **Acknowledgements**

426 We received financial support from the National Science Fund for Distinguished Young  
427 Scholars (41925029), and the National Natural Science Foundation of China (41877125).

428

#### 429 **Competing interests**

430 The authors declare no competing interests.

431

#### 432 **Data availability**

433 The data that support the findings of this study are available from the corresponding  
434 author upon reasonable request.

435

#### 436 **Additional information**

437 Supplementary information is available for this paper at

438

439 **References**

- 440 Abbas, A., Brimer, A., Slocik, J.M., Tian, L., Naik, R.R., Singamaneni, S., 2013. *Anal.*  
441 *Chem.* 85, 3977–3983.
- 442 Aga, D.S., Lenczewski, M., Snow, D., Muurinen, J., Sallach, J.B., Wallace, J.S., 2016. *J.*  
443 *Environ. Qual.* 45, 407–419.
- 444 Ahmed, A., Rushworth, J.V., Hirst, N.A., Millner, P.A., 2014. *Clin. Microbiol. Rev.* 27,  
445 631–646.
- 446 Arefev, K.M., Guseva, M.A., Khomchenkov, B.M., 1987. *High Temp+*. 25, 250–255.
- 447 Bartelt-Hunt, S., Snow, D.D., Damon-Powell, T., Miesbach, D., 2011. *J. Contam. Hydrol.*  
448 123, 94–103.
- 449 Batt, A.L., Aga, D.S., 2005. *Anal. Chem.* 77, 2940–2947.
- 450 Belkin, S., 2003. *Curr. Opin. Microbiol.* 6, 206–212.
- 451 Berendonk, T.U., Manaia, C.M., Merlin, C., Fatta-Kassinos, D., Cytryn, E., Walsh, F.,  
452 Bürgmann, H., Sørum, H., Norström, M., Pons, M., 2015. *Nat. Rev. Microbiol.* 13,  
453 310.
- 454 Bergan, T., Oydvin, B., Lunde, I., 1973. *Pharmacol. Toxicol.* 33, 138–156.
- 455 Burrows, J., Watson, K., 2015. *Bioanalysis* 7, 1731–1743.
- 456 Chaiyo, S., Siangproh, W., Apilux, A., Chailapakul, O., 2015. *Anal. Chim. Acta* 866,  
457 75–83.
- 458 Cipullo, S., Prpich, G., Campo, P., Coulon, F., 2018. *Sci. Total. Environ.* 615, 708–723.
- 459 Du, L., Liu, W., 2012. *Agron. Sustain. Dev.* 32, 309–327.

460 Ferreira, D.C.M., Giordano, G.F., Soares, C.C.D.S., de Oliveira, J.F.A., Mendes, R.K.,  
461 Piazzetta, M.H., Gobbi, A.L., Cardoso, M.B., 2015. *Talanta* 141, 188–194.

462 Gao, Q., Li, Y., Qi, Z., Yue, Y., Min, M., Peng, S., Shi, Z., Gao, Y., 2018. *Sci. Total.*  
463 *Environ.* 630, 117–125.

464 Gothwal, R., Shashidhar, T., 2015. *CLEAN-Soil Air Water* 43, 479–489.

465 Gu, Y., Shen, S., Han, B., Tian, X., Yang, F., Zhang, K., 2020. *Ecotox. Environ. Safe.* 197,  
466 110567.

467 Gullapalli, H., Vemuru, V.S.M., Kumar, A., Botello-Mendez, A., Vajtai, R., Terrones, M.,  
468 Nagarajiah, S., Ajayan, P.M., 2010. *Small* 6, 1641–1646.

469 Hamscher, G., Pawelzick, H.T., Höper, H., Nau, H., 2005. *Environ. Toxicol. Chem* 24,  
470 861–868.

471 Hamscher, G., Sczesny, S., Höper, H.A., Heinz, N., 2002. *Anal. Chem.* 74, 1509–1518.

472 Hansen, L.H., Sørensen, S.J., 2001. *Microbial Ecol.* 42, 483–494.

473 Hoa, P.T.P., Managaki, S., Nakada, N., Takada, H., Shimizu, A., Anh, D.H., Viet, P.H.,  
474 Suzuki, S., 2011. *Sci. Total. Environ.* 409, 2894–2901.

475 Hossain, S.M.Z., Luckham, R.E., Smith, A.M., Lebert, J.M., Davies, L.M., Pelton, R.H.,  
476 Filipe, C.D.M., Brennan, J.D., 2009. *Anal. Chem.* 81, 5474–5483.

477 Hu, X., Zhou, Q., Luo, Y., 2010. *Environ. Pollut.* 158, 2992–2998.

478 Iglesias, A., López, R., Gondar, D., Antelo, J., Fiol, S., Arce, F., 2009. *Chemosphere* 76,  
479 107–113.

480 Ikehata, K., Bressler, D., Singh, P., Kaddah, M., El-Din, M.G., 2006. *Water Environ. Res.*



481 78, 1525–1562.

482 Kumar, K., Gupta, S.C., Baidoo, S.K., Chander, Y., Rosen, C.J., 2005. *J. Environ. Qual.*  
483 34, 2082–2085.

484 Li, Y., Wang, H., Liu, X., Zhao, G., Sun, Y., 2016. *Environ. Sci. Pollut. R* 23,  
485 13822–13831.

486 Liana, D.D., Burkhard, R., J Justin, G., Edith, C., 2012. *Sensors-Basel* 12, 11505.

487 Limbu, S.M., Zhou, L., Sun, S., Zhang, M., Du, Z., 2018. *Environ. Int.* 115, 205–219.

488 Liu, B., Li, Y., Zhang, X., Wang, J., Gao, M., 2014. *Soil Biol. Biochem.* 74, 148–155.

489 Liu, F., Ying, G., Tao, R., Zhao, J., Yang, J., Zhao, L., 2009. *Environ. Pollut.* 157,  
490 1636–1642.

491 Liu, S., Zhao, H., Lehmler, H., Cai, X., Chen, J., 2017. *Environ. Sci. Technol.* 51,  
492 2392–2400.

493 Liu, X., Steele, J.C., Meng, X., 2017. *Environ. Pollut.* 223, 161–169.

494 Ma, Z., Liu, J., Li, H., Zhang, W., Williams, M.A., Gao, Y., Gudda, F.O., Lu, C., Yang, B.,  
495 Waigi, M.G., 2020. *Environ. Sci. Technol.* 54, 758–767.

496 Ornatska, M., Sharpe, E., Andreescu, D., Andreescu, S., 2011. *Anal. Chem.* 83,  
497 4273–4280.

498 Orth, P., Schnappinger, D., Hillen, W., Saenger, W., Hinrichs, W., 2000. *Nat. Struct. Biol.*  
499 7, 215–219.

500 Parlanti, E., Wörz, K., Geoffroy, L., Lamotte, M., 2000. *Org. Geochem.* 31, 1765–1781.

501 Peak, N., Knapp, C.W., Yang, R.K., Hanfelt, M.M., Smith, M.S., Aga, D.S., Graham,

- 502 D.W., 2007. *Environ. Microbiol.* 9, 143–151.
- 503 Quesada-González, D., Merkoçi, A., 2015. *Biosens. Bioelectron.* 73, 47–63.
- 504 Rico, A., Jacobs, R., Van den Brink, P.J., Tello, A., 2017. *Environ. Pollut.* 231, 918–928.
- 505 Rodriguez-Mozaz, S., Chamorro, S., Marti, E., Huerta, B., Gros, M., Sànchez-Melsió, A.,  
506 Borrego, C.M., Barceló, D., Balcázar, J.L., 2015. *Water Res.* 69, 234–242.
- 507 Sambrook, J., Fritsch, E.F., Maniatis, T., 1989. *Molecular cloning: a laboratory manual.*  
508 Cold Spring Harbor Laboratory.
- 509 Scarano, C., Piras, F., Viridis, S., Ziino, G., Nuvoloni, R., Dalmaso, A., De Santis, E.P.L.,  
510 Spanu, C., 2018. *Int. J. Food Microbiol.* 284, 91–97.
- 511 Struss, A., Pasini, P., Ensor, C.M., Raut, N., Daunert, S., 2010. *Anal. Chem.* 82,  
512 4457–4463.
- 513 Teuber, M., 2001. *Curr. Opin. Microbiol.* 4, 493–499.
- 514 Thiele-Bruhn, S., 2003. *J. Plant Nutr. Soil Sc.* 166, 145–167.
- 515 Wang, W., Wu, W., Wang, W., Zhu, J., 2010. *J. Chromatogr. A* 1217, 3896–3899.
- 516 Zhu, J., Snow, D.D., Cassada, D.A., Monson, S.J., Spalding, R.F., 2001. *J. Chromatogr. A*  
517 928, 177–186.
- 518 Zhu, Y., Johnson, T.A., Su, J., Qiao, M., Guo, G., Stedtfeld, R.D., Hashsham, S.A., Tiedje,  
519 J.M., 2013. *P. Natl. Acad. Sci. Usa.* 9, 3435–3440.
- 520 Zilles, J., Shimada, T., Jindal, A., Robert, M., Raskin, L., 2005. *Water Environ. Res.* 77,  
521 57–62.
- 522 Zou, Y., Zhang, Y., Xu, Y., Chen, Y., Huang, S., Lyu, Y., Duan, H., Chen, Z., Tan, W.,

523 2018. *Anal. Chem.* 90, 13687–13694.